

MAY 01 2006

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130174

Name Steve Christensen ID# 1315 Date 4/25/06

A Agency Juneau Police Dept Phone # 907-586-0600

Instrument Location Juneau Police

B Alco S/N X301540 Target Value .082 High Pressure 1150

Alco Test Value Average .083 .084

1st Alco 2nd Alco

Signature [Signature] C.O.B. 5/2/06

(OVER)


Under the Alaska Rules of Evidence, I ^(Do Not write in the area below) certify that,

(a) I am Chris W. Beheim, Director, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve Christensen, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

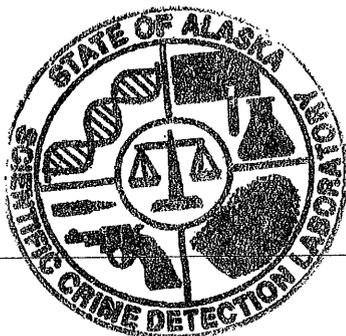

Chris W. Beheim 5-8-06

Chris W. Beheim Date
 Scientific Director
 State of Alaska
 State Breath Alcohol Testing Program

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130174

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

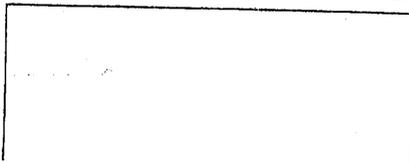

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130174

APRIL 25, 2006

OPERATOR'S NAME:

CHRISTENSEN, S, E

OPERATOR'S NUMBER: 1315

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :
VOC

O.L. #: 042506

DEPT/AGENCY: JNU1

CASE/REPORT: 042506


TEST TYPE: V

ALCO TARGET VALUE: .082


ALCO S/N: X301540

--- BREATH ANALYSIS ---

.082 ADJUSTED FOR 30.37 in
ALCO TARGET .083 03:41
BLANK TEST .000 03:43
INTERNAL STANDARD VERIFIED 03:43
ALCO TV 30.37 in .083 03:43
BLANK TEST .000 03:44
SUBJECT SAMPLE .000 03:45
BLANK TEST .000 03:45
ALCO TV 30.37 in .084 03:46
BLANK TEST .000 03:47

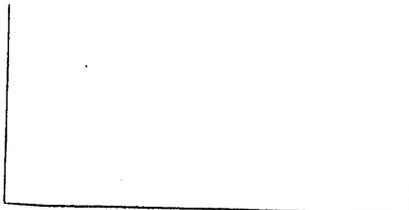

DIAGNOSTIC CHECK



ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130174

APRIL 25, 2006

TIME 03:47

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 40c
BAROMETER: 30.37 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNOPQRSTUVWXYZ[\]^_`abcdefghijklmnopqr
stuvwxyz{|}~*~

