

VERIFICATION OF CALIBRATION REPORT JAN 23 2012

of DataMaster cdm Breath Test Instrument
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

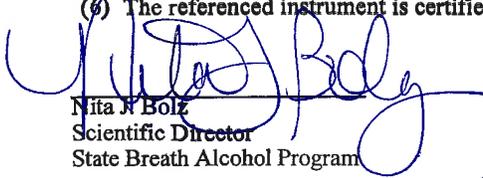
DataMaster cdm S/N <u>130176</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>DARYL RICE</u>	ID# <u>2088</u> Date <u>01/14/2012</u>
A Agency <u>SITKA POLICE DEPT.</u> Phone # <u>747-3245</u>	
Instrument Location <u>304 LAKE STREET</u>	
B Alco S/N <u>X172969</u> Target Value <u>.077</u> High Pressure <u>800</u>	
Alco Test Values	<u>.081</u> <u>.081</u>
1st Alco	2 nd Alco
Signature <u>Daryl Rice</u>	<u>CRB</u> <u>1/23/12</u>

(OVER)

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Feb 2012 CRB


(Notary Seal Stamp)
Daniel L. Nicholas Nikki Roth
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130176

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

COB/23/12
ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130176

JANUARY 14, 2012

OPERATOR'S NAME:
RICE DARYL DEAN
OPERATOR'S NUMBER: 2888
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
VOC

D.L. #: VOC
DEPT/AGENCY: SIT1
CASE/REPORT: VOC
TEST TYPE: U
ALCO TARGET VALUE: .877
ALCO S/N: X172959

— BREATH ANALYSIS —

.877 ADJUSTED FOR 30.20 in
ALCO TARGET .877 06:33
BLANK TEST .880 06:34
INTERNAL STANDARD VERIFIED 06:34
ALCO TV 30.20 in .881 06:35
BLANK TEST .880 06:36
SUBJECT SAMPLE .880 06:36
BLANK TEST .880 06:37
ALCO TV 30.20 in .881 06:37
BLANK TEST .880 06:38

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130176

JANUARY 14, 2012
TIME 06:24

WTC PSC 800
01/14/12
Daryl Rice

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.20 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~ ! ! !