

FEB 02 2011  
2011  
2010-01-31

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130176 ✓

Name DARYL RICE ID# 2088 Date 01/27/11 ✓

A Agency SETKA POLICE DEPT. Phone # 747-3245

Instrument Location 304 LAKE STREET

---

B Alco S/N X301572 ✓ Target Value .078 ✓ High Pressure 550

Alco Test Values .084 ✓ 1st Alco .079 ✓ 2nd Alco

Signature Daryl Rice

(OVER)

(Do Not write in the area below)

*AMB*  
2/8/11


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 8<sup>th</sup> day of MAR, 2011

*Daniel L. Nicholas*  
 (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

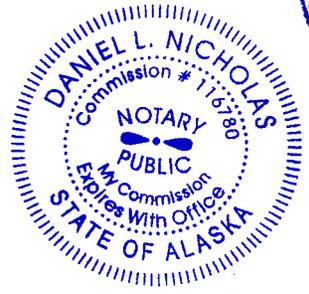

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130176

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130176  
JANUARY 27, 2011  
OPERATOR'S NAME:  
RICE DARYL DEAN  
OPERATOR'S NUMBER: 2888  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
UOC  
O.L. #: UOC  
DEPT/AGENCY: SIT1  
CASE/REPORT: UOC  
TEST TYPE: U  
ALCO TARGET VALUE: .078  
ALCO S/N: K301572

### — BREATH ANALYSIS —

.078 ADJUSTED FOR 30.42 in  
ALCO TARGET .079 09:49  
BLANK TEST .000 09:50  
INTERNAL STANDARD VERIFIED 09:50  
ALCO TU 30.42 in .004 09:50  
BLANK TEST .000 09:51  
SUBJECT SAMPLE .000 09:51  
BLANK TEST .000 09:52  
ALCO TU 30.42 in .079 09:52  
BLANK TEST .000 09:53

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130176  
JANUARY 27, 2011  
TIME 09:53

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.42 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { } ~ |