

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130177 ✓			
Name	SEAN E ADKINS	ID#	S110	Date	4/09/2008 ✓	
A	Agency	ALASKA STATE TROOPERS		Phone #	(907) 438-2029	
	Instrument Location	St. Mary's ✓				
B	Alco S/N	5842B ✓	Target Value	.079 ✓	High Pressure	200 P.S.I.
	Alco Test Values	.082 ✓	.083 ✓	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
	Signature			CUB 4/15/08		
(OVER)						


Under the Alaska Rules of Evidence, I certify that;  
(Do Not write in the area below)


(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Sean Adkins, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

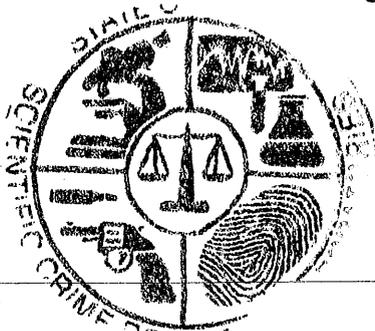



4/20/08

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

Date

APR 14 2008

BT9 03/00

APR 14 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130177

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130177

APRIL 09, 2008

OPERATOR'S NAME:

ADKINS/S/E

OPERATOR'S NUMBER: 5110

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: VOC

DEPT/AGENCY: SMD

CASE/REPORT: VOC

TEST TYPE: U

ALCO TARGET VALUE: .079

ALCO S/N: 58428

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.93 in  
ALCO TARGET .079 16:07  
BLANK TEST .000 16:08  
INTERNAL STANDARD VERIFIED 16:08  
ALCO TV 29.93 in .082 16:08  
BLANK TEST .000 16:09  
SUBJECT SAMPLE .000 16:10  
BLANK TEST .000 16:10  
ALCO TV 29.93 in .083 16:11  
BLANK TEST .000 16:12

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130177

APRIL 09, 2008  
TIME 16:04

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.93 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@ABCDEF  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopq  
rstuvwxyz{|}~

APR 14 2008