

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure: <b>DataMaster cdm S/N</b> <u>130177</u>	
Name <u>SEAN E ADKINS</u>	ID# <u>5110</u> Date <u>6/08/2008</u> ✓
A Agency <u>ALASKA STATE TROOPERS</u> Phone # <u>(907) 438-2029</u>	
Instrument Location <u>ST. Mary's</u> ✓	
B Alco S/N <u>50428</u> ✓ Target Value <u>.079</u> ✓ High Pressure <u>200 P.S.I</u>	
Alco Test Values <u>.083</u> ✓ <u>.081</u> ✓	
1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco	
Signature <u>[Signature]</u> <u>CSB</u> <u>6/20/08</u>	
(OVER)	

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Sean Adkins, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

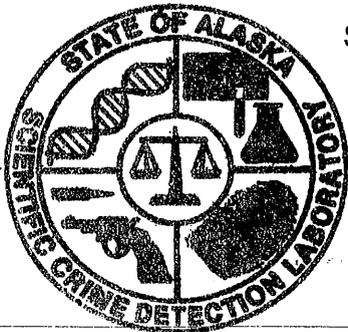

Signed and sealed,

[Signature]

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

6/20/08  
Date

JUN 10 2008

BT9 03/00

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130177

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130177

JUNE 08, 2008 ✓ *CD 6/20/08*

OPERATOR'S NAME:  
ADKINS/S/E  
OPERATOR'S NUMBER: 5110  
SUBJECT'S LAST NAME:  
VERIFICATION OF CALIBRATION  
SUBJECT'S FIRST NAME/NI :  
UOC  
O.L. #: UOC  
DEPT/AGENCY: SAA/0  
CASE/REPORT: UOC  
TEST TYPE: U  
ALCO TARGET VALUE: .079 ✓  
ALCO S/N: 58428 ✓

— BREATH ANALYSIS —

.079 ADJUSTED FOR 29.96 in  
ALCO TARGET .079 09:02  
BLANK TEST .000 09:03  
INTERNAL STANDARD VERIFIED 09:03  
ALCO TU 29.96 in .083 ✓ 09:03  
BLANK TEST .000 09:04  
SUBJECT SAMPLE .000 *CD 6/20/08* 09:04  
BLANK TEST .000 09:05  
ALCO TU 29.96 in .081 ✓ 09:06  
BLANK TEST .000 09:06

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130177

JUNE 08, 2008 ✓  
TIME 08:59

— DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.96 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~