

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130 178</u>
Name	<u>James K. Kimura</u>	ID# <u>5677</u> Date <u>10-17-08</u> ✓
A Agency	<u>Alaska State Troopers</u>	Phone # <u>(907) 225-5118</u>
Instrument Location	<u>Ketchikan AST Post</u> ✓	
B Alco S/N	<u>78820</u> ✓	Target Value <u>.077</u> ✓ High Pressure <u>3,500 PSI</u> ✓
Alco Test Values	<u>.079</u> ✓ 1 <sup>st</sup> Alco	<u>.077</u> ✓ 2 <sup>nd</sup> Alco
Signature	<u>[Signature]</u> ✓ JKK 10/17/08	<u>[Signature]</u> ✓ COB 11/4/08

(OVER)


Under the Alaska Rules of Evidence, I certify that, (Do not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, James Kimura, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

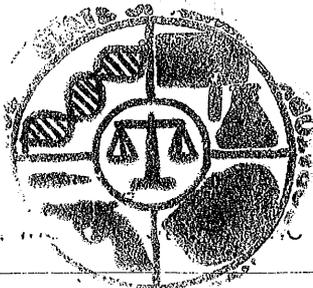

[Signature] 11/5/08  
Date  
Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130 178 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130178

OCTOBER 17, 2008 ✓ *CBS 11/11/08*

OPERATOR'S NAME:  
SUPERVISOR *JKK*  
OPERATOR'S NUMBER: 5677  
SUBJECT'S LAST NAME:  
KINURA  
SUBJECT'S FIRST NAME/MI :  
JAMES/K

O.L. #: 000000  
DEPT/AGENCY: KETO  
CASE/REPORT: 00-0000000  
TEST TYPE: U  
ALCO TARGET VALUE: .077 ✓  
ALCO S/N: 78820 ✓

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 30.04 in  
ALCO TARGET .077 17:40  
BLANK TEST .000 17:41  
INTERNAL STANDARD VERIFIED 17:41  
ALCO TV 30.04 in .079 17:41  
BLANK TEST .000 17:42  
SUBJECT SAMPLE .000 17:42  
BLANK TEST .000 17:43  
ALCO TV 30.04 in .077 17:44  
BLANK TEST .000 17:44

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130178

OCTOBER 17, 2008 ✓  
TIME 17:26

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.03 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! "#\$%&'()\*+,-./0123456789:;<=>@ABCDEFGHIJK  
LMNOPQRSTUVWXYZ[\]^\_`abcde fghijklmnop  
qrstuvwxyz{|}~#