


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

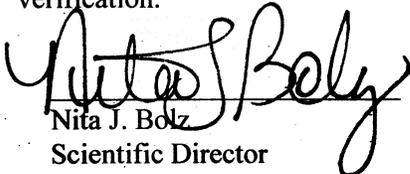
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

APR 22 2009


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130179 ✓			
Name	John T. Ostoj	ID#	4823			
		Date	4/20/09 ✓			
A	Agency	Soldotna AST	Phone # <u>512.09</u>			
	Instrument Location	Soldotna AST ✓				
Alco S/N		X301540 ✓	Target Value	.082 ✓	High Pressure	1100
B		Alco Test Value Average	.082 ✓	.082 ✓		
		1 st Alco		2 nd Alco		
Signature						
(OVER)						


I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 22 day of May, 2009.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130179 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATA MASTER cdm 130179

APRIL 20, 2009 ✓

OPERATOR'S NAME:

OSTOJ/JOHN/T

OPERATOR'S NUMBER: 4827

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

TEST

CELL #: UOC

DEPT/AGENCY: SLDG

OFFICE/REPORT: UOC

TEST TYPE: U

ALCOHOL TARGET VALUE: .002 ✓

--- BREATH ANALYSIS ---

ALCOHOL ADJUSTED FOR 30.27 in		
ALCOHOL TARGET	.002	07:10
BLANK TEST	.000	07:12
INTERNAL STANDARD	VERIFIED	07:12
ALCOHOL TV 30.27 in	.002	07:12 ✓
BLANK TEST	.000	07:13
SUBJECT SAMPLE	.000	07:14
BLANK TEST	.000	07:14 ✓
ALCOHOL TV 30.27 in	.002	07:15
BLANK TEST	.000	07:16

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATA MASTER cdm 130179

APRIL 20, 2009 ✓

TIME 07:20

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

SEALERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 30.27 in

LOW DETECTOR: OKAY

FLOW SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF6
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~■