

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130179 ✓

Supervisor/Operator Performing the Verification Procedure:

Name V. Eugene Fowler ID# 4386 ✓ Date 10-1-10 ✓

A Agency Alaska State Troopers Phone # \_\_\_\_\_

Instrument Location Soldotna AST Post

---

B Alco S/N X301553 ✓ Target Value .081 ✓ High Pressure 1200

Alco Test Value Average .078 ✓ .077 ✓  
 1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature V E Fowler

(OVER)

*BMB*  
*12/9/10*

*mailed  
on 11/2/10  
V.E.F.*


I, Nita J. Bolz, after being first duly sworn, depose and state as follows (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

*Nita J. Bolz*  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 16<sup>th</sup> day of DEC, 2010.

*[Signature]* (Notary Seal Stamp)  
 Daniel L. Nicholas  
 Notary Public, State of Alaska  
 Commission Expires with Office

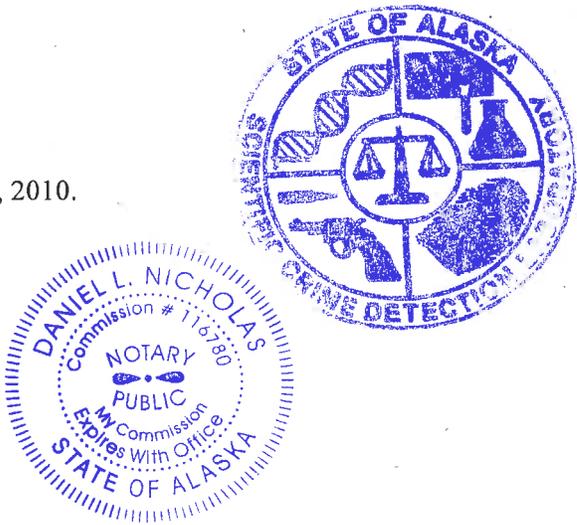

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130179

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

NOVEMBER 01, 2010

OPERATOR'S NAME:  
FOWLER/W/E

OPERATOR'S NUMBER: 4386

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :  
VOC

O.L. #: VOC

DEPT/AGENCY: SLT5

CASE/REPORT: VOC

TEST TYPE: U

ALCO TARGET VALUE: .001

ALCO S/N: X301553

### — BREATH ANALYSIS —

.001 ADJUSTED FOR 28.94 in  
ALCO TARGET .078 15:43  
BLANK TEST .000 15:44  
INTERNAL STANDARD VERIFIED 15:44  
ALCO TV 28.94 in .078 15:44  
BLANK TEST .000 15:45  
SUBJECT SAMPLE .000 15:46  
BLANK TEST .000 15:46  
ALCO TV 28.94 in .077 15:47  
BLANK TEST .000 15:48

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130179

NOVEMBER 01, 2010  
TIME 15:37

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 40c

BAROMETER: 28.92 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { } ~ |