

VERIFICATION OF CALIBRATION REPORT 1

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		Datamaster cdm S/N	130180 ✓
Name		A. W. Anderson	ID# 24967 Date 01/27/2009
A	Agency	Seldovia Police Dept.	Phone # _____
Instrument Location		Seldovia Police Dept. ✓	
Alco S/N		X 301530 ✓	Target Value .078 High Pressure 100 PSI ✓
B	Alco Test Value Average	.075 ✓	.075 ✓
		1 st Alco	2 nd Alco
Signature		A W Anderson ✓	CSB 2/9/09

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, A W Anderson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

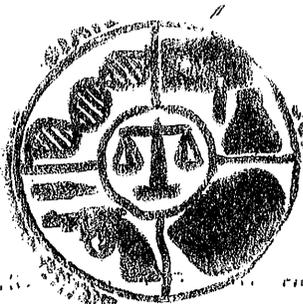

Signed and sealed,

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

2/9/09
Date

BT9 01/00

JAN 30 2009

VERIFICATION OF CALIBRATION REPORT

of Datamaster cdm

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Datamaster cdm S/N 130180

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

JANUARY 27, 2009 ✓ *CB 2/1/09*

OPERATOR'S NAME:
ANDERSON, RW
OPERATOR'S NUMBER: 2467
SUBJECT'S LAST NAME:
VERIFICATION OF CALIBRATION
SUBJECT'S FIRST NAME/MI :
N/A

O.L. #: 1234567890
DEPT/AGENCY: SOVI
CASE/REPORT: N/A
TEST TYPE: U

ALCO TARGET VALUE: .078 ✓
ALCO S/N: X301530

--- BREATH ANALYSIS ---

.078 ADJUSTED FOR 29.90 in

ALCO TARGET	.077	15:00
BLANK TEST	.000	15:01
INTERNAL STANDARD	VERIFIED	15:01
ALCO TV 29.90 in	.075 ✓	15:02
BLANK TEST	.000	15:03
SUBJECT SAMPLE	.000 <i>CB 2/1/09</i>	15:03
BLANK TEST	.000	15:04
ALCO TV 29.91 in	.075 ✓	15:04
BLANK TEST	.000	15:05

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

JANUARY 27, 2009 ✓
TIME 14:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.90 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJK
LMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~@