

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130181

Supervisor/Operator Performing the Verification Procedure:
Name Randy Simons ID# 5123 Date 3-28-12

A Agency AST Phone # 320-6166

Instrument Location Nenana

B Alco S/N ~~xx~~ 4x ^{BMB} 4/2/12 Target Value .080 High Pressure 750

Alco Test Values .079 .079
1st Alco 2nd Alco

Signature [Signature] RAS

(OVER)

BMB
4/2/12

(Do Not write in the area below)



I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 5 day of April, 2012. [Signature] 4/5/12

[Signature] (Notary Seal Stamp)
Daniel L. Nicholas Nikki Roth
Notary Public, State of Alaska
Commission Expires with Office

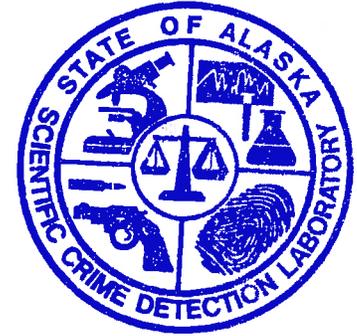

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130181

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130181

MARCH 28, 2012

OPERATOR'S NAME: SIMMONS/ROMMYA
OPERATOR'S NUMBER: 5123
SUBJECT'S LAST NAME: VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI: A
O.L. #: 1
DEPT/AGENCY: MEMO
CASE/REPORT: 1
TEST TYPE: V
ALCO TARGET VALUE: .000
ALCO S/N: 4X

4/2/12

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.00 in		
ALCO TARGET	.077	12:59
BLANK TEST	.000	13:00
INTERNAL STANDARD	VERIFIED	13:00
ALCO TV 29.00 in	.079	13:00
BLANK TEST	.000	13:01
SUBJECT SAMPLE	.000	13:01
BLANK TEST	.000	13:01
ALCO TV 29.10 in	.079	13:02
BLANK TEST	.000	13:02
	.079	13:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130181

MARCH 28, 2012
TIME 13:04

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	42c
BAROMETER:	29.10 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJ KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~