

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130181 ✓
Name	C. RITALA	ID#	3791
		Date	2/12/08
A	Agency		Phone # 786.2640
	A.P.D.		
	Instrument Location		ANCHORAGE JAIL
Alco S/N		Target Value	High Pressure
75602 ✓		085 ✓	1100
Alco Test Values			
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
	084	083	
Signature	Celn Ritala / 1349		083 3/11/08

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

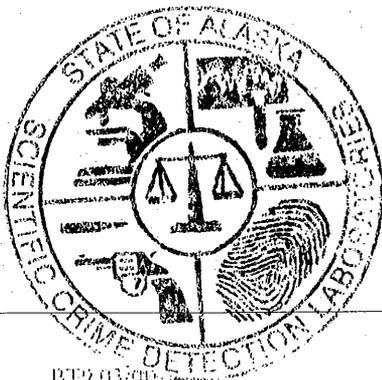

Juanas

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/12/08  
Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130181

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

FEBRUARY 12, 2008

OPERATOR'S NAME:

RITALA

OPERATOR'S NUMBER: 3791

SUBJECT'S LAST NAME:

VERIFICATION OF CALIBRATION

SUBJECT'S FIRST NAME/MI :

A

O.L. #: A

DEPT/AGENCY: ANCI

CASE/REPORT: A

TEST TYPE: V

ALCO TARGET VALUE: 005

ALCO S/N: 75602

--- BREATH ANALYSIS ---

.005 ADJUSTED FOR 29.88 in		
ALCO TARGET	.004	21:30
BLANK TEST	.000	21:31
INTERNAL STANDARD	VERIFIED	21:31
ALCO TV 29.88 in	.004	21:31
BLANK TEST	.000	21:32
SUBJECT SAMPLE	.000	21:33
BLANK TEST	.000	21:34
ALCO TV 29.90 in	.003	21:34
BLANK TEST	.000	21:35

CR 1349 2/12/08

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130181

FEBRUARY 12, 2008

TIME 21:27

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.88 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z ! " #

CR 1349  
2/12/08