

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

SEP 10 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130182
Name	J Swartz	ID#	4314
		Date	5/8/09
A	Agency	SCDL	Phone # 269-5592
	Instrument Location	SCDL	
B	Alco S/N	SCOTT 08	Target Value .080
			High Pressure 800 psi
	Alco Test Values	.078	.078
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
	Signature	J Swartz	

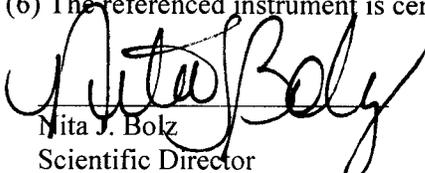
(OVER)

BMB  
9/10/09

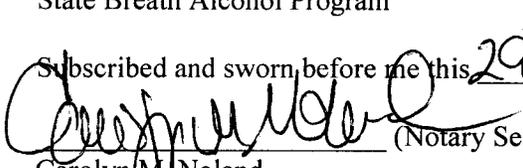
(Do Not write in the area below)

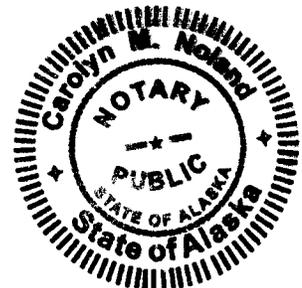
I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 29<sup>th</sup> day of Sept., 2009.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

MAY 08, 2009

OPERATOR'S NAME:  
SWARTZ/J

OPERATOR'S NUMBER: 4314

SUBJECT'S LAST NAME:

VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: AAA1

CASE/REPORT:

TEST TYPE: U

ALCO TARGET VALUE: .000 ✓

ALCO S/N: SCOTT08 ✓

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.32 in ✓  
ALCO TARGET .001 17:23  
BLANK TEST .000 17:23  
INTERNAL STANDARD VERIFIED 17:23  
ALCO TV 30.32 in .078 17:24  
BLANK TEST .000 17:25  
SUBJECT SAMPLE .000 17:25  
BLANK TEST .000 17:26  
ALCO TV 30.32 in .078 17:26  
BLANK TEST .000 17:27

5/8/09

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

MAY 08, 2009 ✓  
TIME 17:21 ✓

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.32 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~