

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JUN 21 2010

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130182</u> ✓
Name	<u>JOHN BENNETT</u>	ID#	<u>4084</u> ✓
		Date	<u>6-19-10</u> ✓
A	Agency	<u>APD</u>	Phone # <u>786-8645</u>
	Instrument Location	<u>ANCHORAGE JAIL</u>	
B	Alco S/N	<u>58428</u> ✓	Target Value <u>.084</u> ✓
		High Pressure	<u>800</u>
	Alco Test Values	<u>.087</u> ✓	<u>.088</u> ✓
		1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
	Signature		

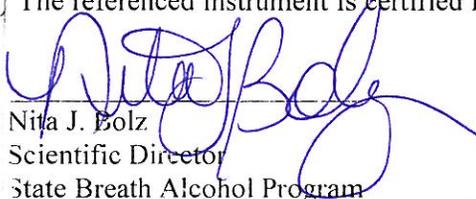
(OVER)

(Do Not write in the area below)

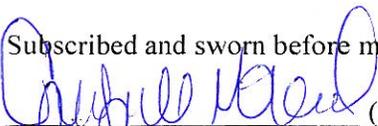
BMB  
6/23/10


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21<sup>st</sup> day of July, 2010.

  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

JUNE 19, 2010

OPERATOR'S NAME:

BENNETT, JOHN

OPERATOR'S NUMBER: 4084

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: 1234567

DEPT/AGENCY: ANCI

CASE/REPORT: 10-VOC

TEST TYPE: V

ALCO TARGET VALUE: .084

ALCO S/N: 58428

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.29 in  
ALCO TARGET .085 09:50  
BLANK TEST .000 09:52  
INTERNAL STANDARD VERIFIED 09:52  
ALCO TV 30.29 in .087 09:52  
BLANK TEST .000 09:53  
SUBJECT SAMPLE .000 09:53  
BLANK TEST .000 09:54  
ALCO TV 30.29 in .088 09:54  
BLANK TEST .000 09:55

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

JUNE 19, 2010

TIME 09:56

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 30.29 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! "\$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ Δ