

CDW  
8-26-09

AUG 8 0 9N

~~JUL 28 2009~~

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 ✓

Supervisor/Operator Performing the Verification Procedure:

Name SERGEANT JAMES MICHELS ID# 6502 Date 8/3/09 ✓

A Agency USIB POLICE DEPT Phone # 852-6111

Instrument Location BARROW, USIBPD, SQUAD ROOM ✓

---

B Alco S/N X 301568 ✓ Target Value .084 ✓ High Pressure 1300 psc

Alco Test Values .086 ✓ .086 ✓  
                                   1<sup>st</sup> Alco                                    2<sup>nd</sup> Alco

Signature SGT James Michels 575 ✓ COB  
8/17/09

(OVER)

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of August, 2009.

Carolyn M. Noland (Notary Seal Stamp)  
 Carolyn M. Noland  
 Notary Public, State of Alaska  
 Commission Expires with Office

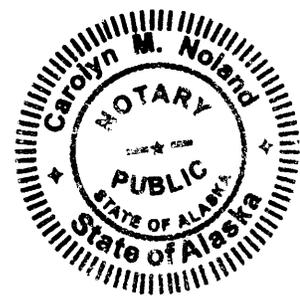

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

AUGUST 03, 2009

OPERATOR'S NAME:

MICHELIS/JAMES

OPERATOR'S NUMBER: 6502

SUBJECT'S LAST NAME:

UOC

SUBJECT'S FIRST NAME/MI :

UOC

O.L. #: UOC

DEPT/AGENCY: BRW1

CASE/REPORT: UOC

TEST TYPE: U

ALCO TARGET VALUE: .084 ✓

ALCO S/N: X301568 ✓

### --- BREATH ANALYSIS ---

.084 ADJUSTED FOR 30.43 in ✓  
ALCO TARGET .085 18:58  
BLANK TEST .000 18:59  
INTERNAL STANDARD VERIFIED 18:59  
ALCO TV 30.43 in .086 ✓ 18:59  
BLANK TEST .000 19:00  
SUBJECT SAMPLE .000 19:00  
BLANK TEST .000 19:01  
ALCO TV 30.43 in .086 ✓ 19:02  
BLANK TEST .000 19:02

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

AUGUST 03, 2009 ✓

TIME 18:42

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.43 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!\*"#%&'()\*+,-./0123456789:;<=>@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~■