

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130182</u> ✓
Name	<u>Tim Tuckwood</u>	ID#	<u>3446</u> Date <u>10-26-08</u> ✓
A Agency	<u>Alaska State Troopers</u>	Phone #	<u>895-4800</u>
Instrument Location	<u>Delta Court</u> ✓		
B Alco S/N	<u>X301596</u> ✓	Target Value	<u>.081</u> ✓ High Pressure <u>800</u> ✓
Alco Test Value Average	<u>.079</u> ✓		<u>.080</u> ✓
	1 <sup>st</sup> Alco		2 <sup>nd</sup> Alco
Signature	<u>Tim Tuckwood</u> ✓		<u>CS</u> <u>11/4/08</u>

(OVER)

Under the Alaska Rules of Evidence, I certify that;


(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Tim Tuckwood, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

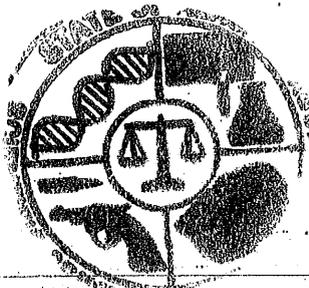

Jeanne Swartz

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

11/5/08

Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

OCTOBER 26, 2008 ✓ *11/1/08*

OPERATOR'S NAME:  
TUCKWOOD TIM  
OPERATOR'S NUMBER: 3446  
SUBJECT'S LAST NAME:  
VERIF  
SUBJECT'S FIRST NAME/MI :  
OF CAL  
O.L. #: 12345  
DEPT/AGENCY: DJTB  
CASE/REPORT: 09876  
TEST TYPE: V  
ALCO TARGET VALUE: .081 ✓  
ALCO S/N: X301596

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.07 in		
ALCO TARGET	.078	13:38
BLANK TEST	.000	13:39
INTERNAL STANDARD	VERIFIED	13:39
ALCO TV 29.07 in	.079	13:40
BLANK TEST	.000	13:40
SUBJECT SAMPLE	.000	13:41
BLANK TEST	.000	13:42
ALCO TV 29.07 in	.080	13:42
BLANK TEST	.000	13:43

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

OCTOBER 26, 2008 ✓  
TIME 13:36

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	43c
BAROMETER:	29.07 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢