

NOV 12 2010

VERIFICATION OF CALIBRATION REPORT

*of DataMaster cdm Breath Test Instrument
State of Alaska*

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130182 ✓
Name		6520 ✓	Date 11-6-10 ^{new} 12/4/10
A	Agency	APD	Phone # 786 8968
Instrument Location ANJ South			
Alco S/N		24 ✓	Target Value 1080 ✓
			High Pressure 1250
Alco Test Values		1st Alco 1079 ✓	2nd Alco 1079 ✓
Signature 			


(OVER)

BMB
12/16/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

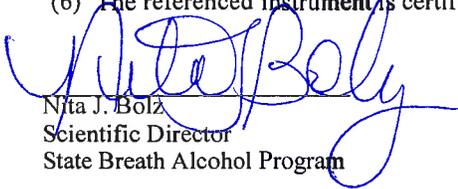

Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 23rd day of DEC, 2010.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

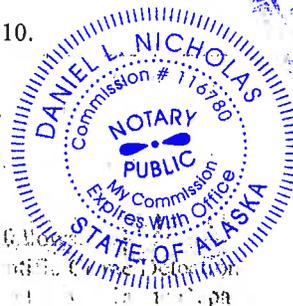

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182 ^{DLW} 12/9/10

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130182

NOVEMBER 06, 2010

OPERATOR'S NAME:

NOLL

OPERATOR'S NUMBER: 6520

SUBJECT'S LAST NAME:

CALIBRATION

SUBJECT'S FIRST NAME/MI :

VERIFICATION/OF

O.L. #: 012345

DEPT/AGENCY: ANCI

CASE/REPORT: 10-98765

TEST TYPE: V

ALCO TARGET VALUE: .080

ALCO S/N: 2U

DN
30210
11-6-10
BMB
12/16/10

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 29.38 in		
ALCO TARGET	.078	04:04
BLANK TEST	.000	04:05
INTERNAL STANDARD	VERIFIED	04:05
ALCO TV 29.38 in	.079	04:05
BLANK TEST	.000	04:06
SUBJECT SAMPLE	.000	04:07
BLANK TEST	.000	04:08
ALCO TV 29.38 in	.079	04:08
BLANK TEST	.000	04:09

BMB
12/16/10

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130182

NOVEMBER 06, 2010

TIME 04:02

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.38 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

DN
30210
11-6-10

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGH
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~Δ

