

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130182 ✓
Name	STEVE DUNN	ID#	4106 ✓
		Date	11-16-10 ✓
A	Agency	APD	Phone # 786-8200
	Instrument Location	ANCHORAGE JAIL	
Alco S/N		2Y ✓	Target Value .080 ✓
			High Pressure 1100
B	Alco Test Values	.081 ✓	.082 ✓
		1st Alco	2nd Alco
Signature			

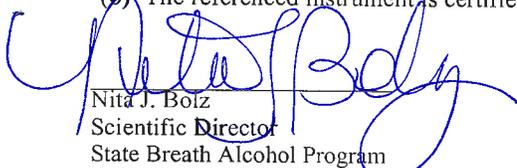
(OVER)

BMB  
12/16/10

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 23<sup>RD</sup> day of DEC, 2010.

  
(Notary Seal Stamp)  
Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130182

*BMB*  
*12/16/10*

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

NOVEMBER 16, 2010

*BMB*  
*12/16/10*

OPERATOR'S NAME:  
DUNN/S  
OPERATOR'S NUMBER: 4106  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
V  
O.L. #: V  
DEPT/AGENCY: ANCI  
CASE/REPORT: V  
TEST TYPE: V  
ALCO TARGET VALUE: .080  
ALCO S/N: 2Y

*S. Dunn*  
*\*1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130182

NOVEMBER 16, 2010  
TIME 13:05

*S. Dunn*  
*\*136*

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.61 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 30.61 in  
ALCO TARGET .081 13:07  
BLANK TEST .000 13:08  
INTERNAL STANDARD VERIFIED 13:08  
ALCO TV 30.61 in .081 13:08  
BLANK TEST .000 13:09  
SUBJECT SAMPLE .000 13:09  
BLANK TEST .000 13:10  
ALCO TV 30.61 in .082 13:10  
BLANK TEST .000 13:11

*BMB*  
*12/16/10*

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqr  
rstuvwxyz{|}~`