

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N 130183	
Name	Hutt, William	ID#	3359
Date	02/20/08		
Agency	Homer Police Dept./Jail		Phone# 235-3150
Instrument Location	4060 Heath St. Homer, AK 99603		
Alco S/N	77180 ✓	Target Value	.081 ✓
High Pressure	800 psi		
Alco Test Value Average	.080	.080	
	1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco	
Signature	William T. Hutt		03/28/08

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, William Hutt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

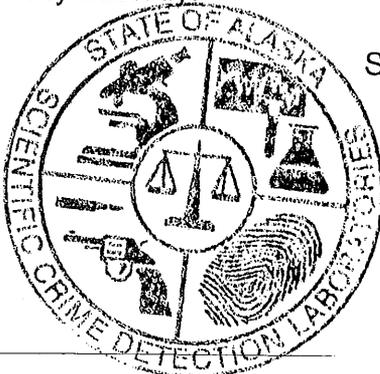

Signed and sealed,

Jeanne Swartz  
Scientific Director Designee  
State of Alaska  
State Breath Alcohol Testing Program

3/1/08

Date

FEB 21 2008

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130183

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130183

FEBRUARY 20, 2008 *WTH*  
*2/26/08*

OPERATOR'S NAME:  
HUTT, WILLIAM T  
OPERATOR'S NUMBER: 3359  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
ETCH

O.L. #: 01234567  
DEPT/AGENCY: HOM1  
CASE/REPORT: 00-0000  
TEST TYPE: V  
ALCO TARGET VALUE: .081  
ALCO S/N: 77180

### --- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.10 in  
ALCO TARGET .078 01:51  
BLANK TEST .000 01:52  
INTERNAL STANDARD VERIFIED 01:52  
ALCO TV 29.10 in .000 01:53  
BLANK TEST .000 01:53  
SUBJECT SAMPLE *WTH* .000 *2/26/08* 01:55  
BLANK TEST .000 *2/26/08* 01:56  
ALCO TV 29.12 in, .000 01:56  
BLANK TEST .000 01:57

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130183

FEBRUARY 20, 2008  
TIME 01:47

*WTH*

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.10 in.  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! "# \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢