

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DEC 04 2010
[Signature]

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130184

Name SGT. JOHN HAMILTON ID# 3192 Date 12/26/09

A Agency PETERSBURG POLICE DEPARTMENT Phone # 772-3888

Instrument Location PETERSBURG ✓

B Alco S/N ~~78268~~ 78268 ^{78/10} ✓ Target Value .081 ✓ High Pressure 425 PSI

Alco Test Values .080 ✓ 1st Alco .080 ✓ 2nd Alco

Signature *[Signature]* ✓

(OVER) *[Signature]*
1/9/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 26th day of January, 2010.

[Signature]
(Notary Seal Stamp)
Carolyn K. Noland
Notary Public, State of Alaska
Commission Expires with Office

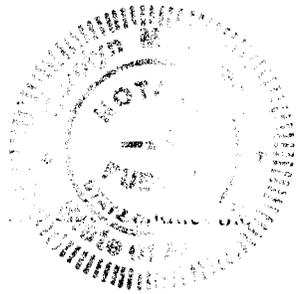

4

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


DataMaster cdm S/N 130184 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

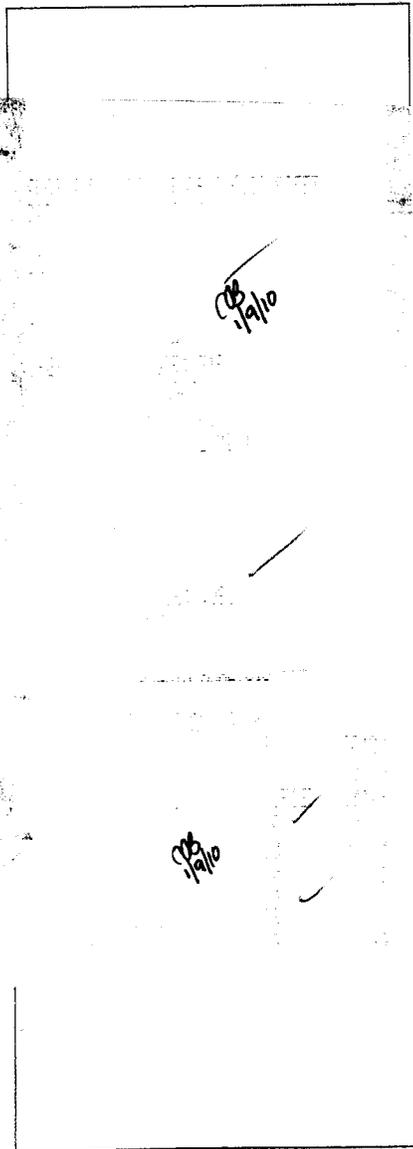

DIAGNOSTIC CHECK

