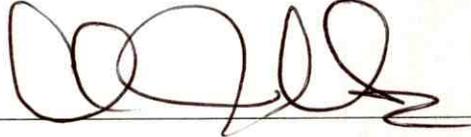


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:	
Name	<u>CHRISTOPHER LIMBS</u> ID# <u>3669</u> Date <u>8/11/12</u>
A Agency <u>ALASKA STATE TROOPERS</u> Phone # <u>465-4004</u>	
Instrument Location <u>BARTUETT COVE, AK</u>	
B Alco S/N <u>2L</u> Target Value <u>.080</u> High Pressure <u>900 PSI</u>	
Alco Test Values <u>.081</u> <u>.081</u> 1st Alco 2 <sup>nd</sup> Alco	
Signature 	
(OVER)	

*AMB*  
*8/16/12*


(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

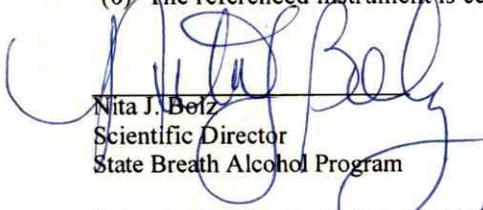  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of Nov, 2012.  
*NAK 11/2/12*

  
(Notary Seal Stamp)  
Daniel L. Nicholas *NIKKI ROTH*  
Notary Public, State of Alaska  
Commission Expires with Office

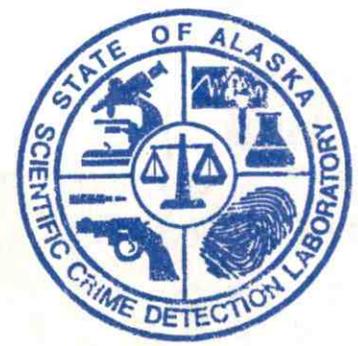

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130185

BMB  
8/11/12

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

AUGUST 11, 2012

OPERATOR'S NAME:

UMBS/CHRISTOPHER/J

OPERATOR'S NUMBER: 3659

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L. #: VOC

DEPT/AGENCY: AST

CASE/REPORT: VOC

TEST TYPE: V

ALCO TARGET VALUE: .030

ALCO S/N: 2L

--- BREATH ANALYSIS ---

.030 ADJUSTED FOR 30.48 in

ALCO TARGET	.031	13:01
BLANK TEST	.000	13:02
INTERNAL STANDARD	VERIFIED	13:02
ALCO TV 30.48 in	.031	13:02
BLANK TEST	.000	13:03
SUBJECT SAMPLE	.030	13:03
BLANK TEST	.000	13:04
ALCO TV 30.48 in	.031	13:04
BLANK TEST	.000	13:05

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

AUGUST 11, 2012

TIME 12:57

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 43c

BREATH TUBE: 43c

BAROMETER: 30.48 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

"#\*X'(+)-.701204\*6789:;<=>@#BCDEFH  
HIJKL"HPQRSTUWXYZ-1" \_'abcde fghijklmno  
pqrstuvwxyz(1)">

