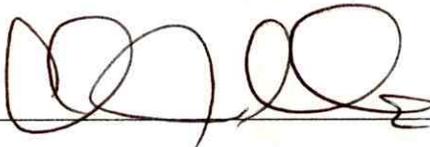


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130185</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>CHRISTOPHER UMBS</u>	ID# <u>3669</u> Date <u>8/31/12</u>
A Agency <u>ALASKA STATE TROOPERS</u>	Phone # <u>465-4000</u>
Instrument Location <u>BARTLETT GVE RANGER STATION - GUSTAVUS</u>	
Alco S/N <u>2L</u> Target Value <u>.080</u> High Pressure <u>850 psi</u>	
B Alco Test Values	<u>.082</u> <u>.082</u> 1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco
Signature	

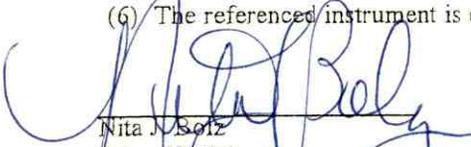
(OVER)

(Do Not write in the area below)


*amb*  
9/10/12

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2nd day of NOV 2012  
*NAK 11/2/12*

 (Notary Seal Stamp)  
Daniel L. Nicholas *Nikki Roth*  
Notary Public, State of Alaska 11/2/12  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N

130185 *BMB 9/10/12*

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

AUGUST 31, 2012

OPERATOR'S NAME: *BMB 9/10/12*  
UMBS/CHRISTOPHER/J  
OPERATOR'S NUMBER: 3659  
SUBJECT'S LAST NAME:

VOC  
SUBJECT'S FIRST NAME/NI :  
VOC

O.L. #: VOC  
DEPT/AGENCY: AST  
CASE/REPORT: VOC  
TEST TYPE: V  
ALCO TARGET VALUE: .030  
ALCO S/N: 2L

--- BREATH ANALYSIS ---

.030 ADJUSTED FOR 30.30 in		
ALCO TARGET	.031	11:59
BLANK TEST	.000	11:00
INTERVAL STANDARD	VERIFIED	11:00
ALCO TV 30.30 in	.032	11:00
BLANK TEST	.000	11:01
SUBJECT SAMPLE	.000	11:02
BLANK TEST	.000	11:02
ALCO TV 30.32 in	.032	11:03
BLANK TEST	.000	11:03

*BMB 9/10/12*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

AUGUST 31, 2012  
TIME 10:50

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	47c
BREATH TUBE:	33c
BAROMETER:	30.32 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#%&'()\*+,-./:0123456789:;<=>?@BCDEFG  
HIJKLMNOPQRSTUVWXYZ\*~\_`abcde fghij<|nop  
pqrstuvwxyz{1}~

