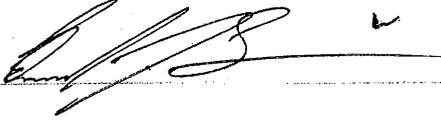



**VERIFICATION OF CALIBRATION REPORT**  
*of DataMaster cdm Breath Test Instrument*  
*State of Alaska*  
*Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program*


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>1300185</u>
Name <u>BRANDON LAWRENSON</u>	ID# <u>66009</u>	Date <u>10/21/08</u> ✓
Agency <u>JUNEAU POLICE DEPT</u>		Phone # <u>586-0600</u>
Instrument Location <u>JUNEAU POLICE DEPT</u> ✓		
B		
Alco S/N <u>X124634</u> ✓	Target Value <u>.081</u> ✓	High Pressure <u>400</u> ✓
Alco Test Values	<u>.088</u> ✓ 1 <sup>st</sup> Alco	<u>.087</u> ✓ 2 <sup>nd</sup> Alco
Signature 		CSB 10/24/08
(OVER)		

Under the Alaska Rules of Evidence, I certify that, (Do Not write in the area below)

- (a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.
- (b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Brandon Lawrenson, whose name appears in my records, is qualified to verify the calibration of the above instrument.
- (c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

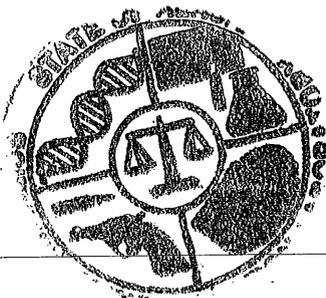



Jeanne Swartz  
 Scientific Director Designee  
 State of Alaska  
 State Breath Alcohol Testing Program

10/29/08  
 Date

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130185 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

OCTOBER 12, 2008 ✓ *COB 10/12/08*

OPERATOR'S NAME:  
LAWRENSON/BRANDON/J  
OPERATOR'S NUMBER: 6609  
SUBJECT'S LAST NAME:  
VOC  
SUBJECT'S FIRST NAME/MI :  
VOC  
O.L. #: 1234567  
DEPT/AGENCY: JNU1  
CASE/REPORT: 0123456  
TEST TYPE: V  
ALCO TARGET VALUE: .081 ✓  
ALCO S/N: X124634

### --- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.22 in		
ALCO TARGET	.081	11:01
BLANK TEST	.000	11:02
INTERNAL STANDARD	VERIFIED	11:02
ALCO TV 30.22 in	.088 ✓	11:02
BLANK TEST	.000	11:03
SUBJECT SAMPLE	.000	11:04
BLANK TEST	.000	11:04
ALCO TV 30.22 in	.087 ✓	11:05
BLANK TEST	.000	11:06

*COB 10/12/08*

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130185

OCTOBER 12, 2008 ✓  
TIME 11:00

### --- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS:	
SAMPLE CHAMBER:	48c
BREATH TUBE:	41c
BAROMETER:	30.22 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
MNOPQRSTUVWXYZ[\]^\_`abcdefghijklmnopqrstuvwxyz{|}~  
~