

VERIFICATION OF CALIBRATION REPORT  
of DataMaster 5005 Breath Test Instrument  
State of Alaska  
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

OCT 26 2010

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130186  
 Name Byron D. Redburn ID# 2087 Date 10-7-10  
 A Agency None PD Phone # 443-5262  
 Instrument Location None PD

---

B Alco S/N X 301548 Target Value .079 High Pressure 200  
 Alco Test Values .081 .081  
 1<sup>st</sup> Alco 2<sup>nd</sup> Alco  
 Signature [Signature]

(OVER)

(Do Not write in the area below)

BMB  
12/8/10

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


[Signature]  
 Nita J. Bolz  
 Scientific Director  
 State Breath Alcohol Program

Subscribed and sworn before me this 16<sup>th</sup> day of DEC, 2010.

[Signature] (Notary Seal Stamp)

Daniel L. Nicholas  
Notary Public, State of Alaska  
Commission Expires with Office

BT9 06/03

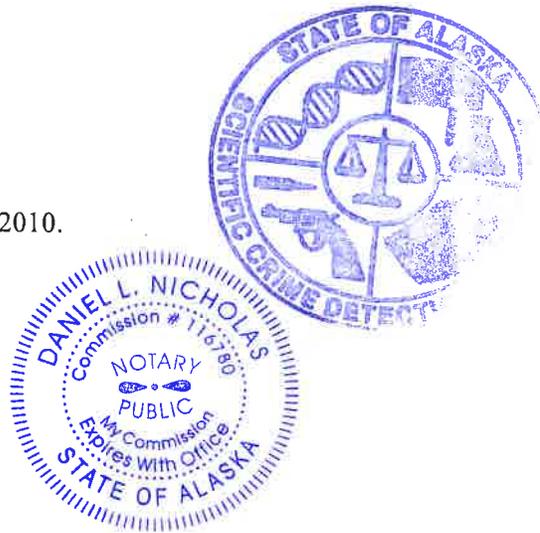

VERIFICATION OF CALIBRATION REPORT

by DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130186

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130186

OCTOBER 07, 2010

OPERATOR'S NAME:  
REGULATORY DIVISION D  
OPERATOR'S NUMBER: 2867  
SUBJECT'S LAST NAME:  
IDENTIFICATION OF DUL  
ELECTRODE TEST NONE/NI :

ALSO TARGET VALUES: .879  
ALSO SNA: 1301549

--- BREATH ANALYSIS ---

ALCOHOL TEST FOR 25.34 in		
ALCOHOL TEST	.879	13:12
ALCOHOL TEST	.880	13:13
ALCOHOL TEST	VERIFIED	13:13
ALCOHOL TEST	.881	13:13
ALCOHOL TEST	.880	13:14
ALCOHOL TEST	.880	13:14
ALCOHOL TEST	.880	13:15
ALCOHOL TEST	.881	13:15
ALCOHOL TEST	.880	13:16

*BMB  
12/8/10*

*BMB  
12/8/10*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130186

OCTOBER 07, 2010  
TIME 13:18

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/09/09

HOSTS:

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETRIC: 29.94 in

FLAME DETECTOR: 3001

ALCOHOL:

ALCOHOL TEST: OKAY

PRINTER TEST

ALCOHOL TEST: OKAY  
ALCOHOL TEST: OKAY  
ALCOHOL TEST: OKAY