


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

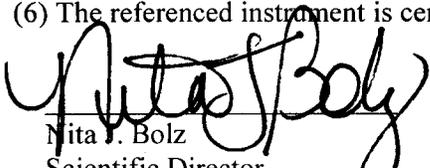
AUG 14 2009

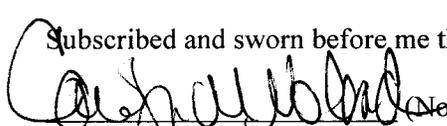
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130187	✓
Name		Dan Pasquariello	ID# 2620	Date 7-31-09 ✓
A	Agency	Dillingham PD	Phone #	842-5354
Instrument Location		Dillingham PD		
Alco S/N		78853 ✓	Target Value	.083 ⁰⁸³ ₈₋₁₄₋₀₉ ✓
			High Pressure	1000 psi
B	Alco Test Value Average	.082 ✓	.082 ✓	
		1 st Alco	2 nd Alco	
Signature			✓	
(OVER)				

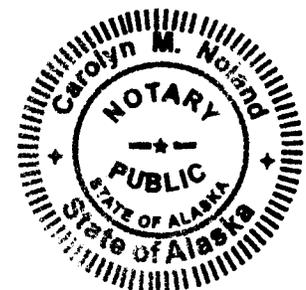
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 17th day of Sept, 2009.

(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130187 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187 ✓

JULY 31, 2009

OPERATOR'S NAME: PASQUARIELLO, DAN
OPERATOR'S NUMBER: 2620
SUBJECT'S LAST NAME: UOR
SUBJECT'S FIRST NAME/MI: UOR
O.I.L. #: 1234567890
DEPT/AGENCY: DL61
CASE/REPORT: 1234567890
TEST TYPE: U
ALCO TARGET VALUE: .083 ✓
ALCO S/N: 78853 ✓

--- BREATH ANALYSIS ---

.083 ADJUSTED FOR 30.24 in ✓
ALCO TARGET .083 12:19
BLANK TEST .000 12:20
INTERNAL STANDARD VERIFIED 12:20
ALCO TU 30.24 in .082 ✓ 12:21
BLANK TEST .000 12:21
SUBJECT SAMPLE .000 12:22
BLANK TEST .000 ✓ 12:23
ALCO TU 30.24 in .082 12:23
BLANK TEST .000 12:24

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130187

JULY 31, 2009 ✓
TIME 12:26

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 48c
BREATH TUBE: 41c
BAROMETER: 30.24 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!""\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcdefghijklmnopqrstuvwxyz{|}~