

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

MAR 11 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130188</u>
A	Name	<u>Hutt, William T.</u>	ID# <u>3359</u> Date <u>03/08/09</u>
	Agency	<u>AST/Anchor Point Post (ANPE)</u>	Phone # <u>235-8239</u>
	Instrument Location	<u>34115 Sterling Hwy./P.O. Box 807</u>	<u>Anchor Point, AK 99556</u>
B	Alco S/N	<u>X301536</u> ✓	Target Value <u>.075</u> High Pressure <u>350 psi</u>
	Alco Test Value Average	<u>.078</u> 1 st Alco	<u>.078</u> 2 nd Alco
	Signature	<u>William T. Hutt</u>	<u>CS</u> <u>3/24/09</u>

(OVER)


(Do Not write in the area below)

Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, William Hutt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

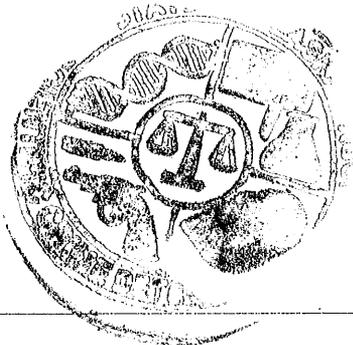

Signed and sealed,

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/24/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130188

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188
MARCH 08, 2009
OPERATOR'S NAME: HUTT, WILLIAM T
OPERATOR'S NUMBER: 3359
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
ETOH
O.L. #: 01234567
DEPT/AGENCY: ASTO / ANPE
CASE/REPORT: 09-00000
TEST TYPE: U
ALCO TARGET VALUE: .075
ALCO S/N: X301536

COB 3/24/09

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 30.63 in	.076	15:30
ALCO TARGET	.000	15:31
BLANK TEST	.000	15:31
INTERNAL STANDARD VERIFIED		15:31
ALCO TU 30.63 in	.078	15:32
BLANK TEST	.000	15:33
SUBJECT SAMPLE	.000	15:34
BLANK TEST	.000	15:34
ALCO TU 30.63 in	.078	15:35
BLANK TEST	.000	15:36

COB 3/24/09

WTH 3/24/09

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188
MARCH 08, 2009
TIME: 15:26
WTH 3/24/09

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/28/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	30.63 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

! " # \$ % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~