

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130180
Name	HUTT, William T.	ID#	3359
Date	05/04/10		
A Agency	AST/Anchor Point Post (ANPE)	Phone #	235-8239 235-3000
Instrument Location	34115 Sterling Hwy/PO Box 807 Anchor Point, AK 99556		
B Alco S/N	X124635	Target Value	0.080
High Pressure	1100 psi		
Alco Test Values	.086	.086	
	1 st Alco	2 nd Alco	
Signature	William T. Hutt		CWB 5/24/10
(OVER)			


I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 10th day of June, 2010.

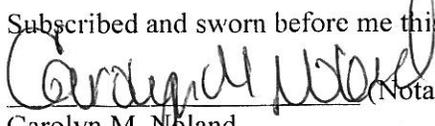
(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130188

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188

MAY 04, 2010

OPERATOR'S NAME: HUTT, WILLIAM T
OPERATOR'S NUMBER: 3359
SUBJECT'S LAST NAME: VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI : ETOH
O.L. #: 01234567
DEPT/AGENCY: AST0 / ANPE
CASE/REPORT: 10-00000
TEST TYPE: U
ALCO TARGET VALUE: 0.080
ALCO S/N: X124635

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 30.66 in
ALCO TARGET .081 04:38
BLANK TEST .080 04:39
INTERNAL STANDARD CO₂ VERIFIED 04:39
ALCO TV 30.66 in 0.086 04:40
BLANK TEST .080 04:41
SUBJECT SAMPLE .080 04:42
BLANK TEST .080 04:43
ALCO TV 30.66 in .086 04:43
BLANK TEST .080 04:44

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188

MAY 04, 2010
TIME 04:34

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.66 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~■