

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument
State of Alaska

MAY 19 2009

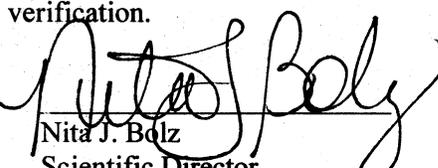
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	132188 ✓
Name		HUTT, William T.	ID# 3359 Date 05/13/09 ✓
A	Agency	AST / Anchor Point Post (ANPE)	Phone # 235-8239 235-3000
Instrument Location		34115 Sterling Hwy. / P.O. Box 007 Anchor Point, AK 99556 ✓	
Alco S/N		X321536 ✓	Target Value .075 ✓
			High Pressure 350 psi
Alco Test Values		.077 ✓	.077 ✓
		1 st Alco	2 nd Alco
Signature		William T. Hutt ✓	
		(OVER)	BMB 5/20/09

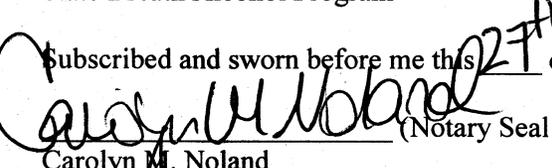
(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 27th day of May 2009.


(Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130188 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188

OPERATOR'S NAME:
MUTT, WILLIAM T
OPERATOR'S NUMBER: 3359
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/NI :
ETOH
O.L. #: 01234567
DEPT/AGENCY: ASTO / ANPE
CASE REPORT: 09-00000
TEST TYPE: V
ALCO TARGET VALUE: ~~0.025~~ 0.075
ALCO S/N: ~~130188~~ X 201586
WTHD

— BREATH ANALYSIS —

ALS ADJUSTED FOR 30.25 in		
ALCO TARGET	.075	00:44
ALCO TEST	.000	00:45
ALCO STANDARD	VERIFIED	00:46
ALCO TU 30.25 in	.077	00:46
ALCO TEST	.000	00:47
ALCO SAMPLE WTHD	.000	00:48
ALCO TEST	.000	00:49
ALCO TU 30.25 in	.077	00:49
ALCO TEST	.000	00:50

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130188

SEP 13, 2009 ✓ WTHD
TIME 00:36

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
STARTUP DATE:	02/20/01
PRINTERS:	
SAMPLE CHANGER:	49c
BREATH TUBE:	42c
BAROMETER:	30.25 in
FLOW DETECTOR:	OKAY
POP	
WHEEL SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST
!"@#\$%^&'()*+,-./0123456789:;<=>?@BCDEFGHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnopqrstuvwxyz{|}~