

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JUL 13 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130189</u> ✓
A	Name	<u>HUTT, William T.</u>	ID# <u>3359</u> Date <u>07/07/09</u>
	Agency	<u>AST/Anchor Point Post (ANPE)</u>	Phone # <u>235-8239</u> <u>235-3000</u>
	Instrument Location	<u>34115 Sterling Hwy./P.O. Box 807 Anchor Point, AK</u> <u>99556</u>	
B	Alco S/N	<u>X301536</u> ✓	Target Value <u>.075</u> ✓ High Pressure <u>350</u> psi
	Alco Test Values	<u>.077</u> ✓ 1 <sup>st</sup> Alco	<u>.070</u> ✓ 2 <sup>nd</sup> Alco
Signature		<u>William T. Hutt</u> ✓	<u>CHB</u> <u>7/14/09</u>
(OVER)			


(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21<sup>st</sup> day of Jul 2009.  
Carolyn M. Noland (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

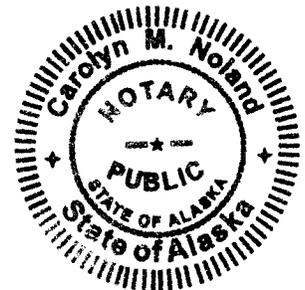

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130188

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130188

JULY 07, 2009 ✓ *CS 7/14/09*

OPERATOR'S NAME:  
MUTT, WILLIAM T  
OPERATOR'S NUMBER: 3359  
SUBJECT'S LAST NAME:  
VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI :  
ETOH  
O.L. #: 01234567  
DEPT/AGENCY: ASTO / ANPE  
CASE/REPORT: 09-00000  
TEST TYPE: U  
ALCO TARGET VALUE: .075 ✓  
ALCO S/N: X301536 ✓

### — BREATH ANALYSIS —

.075 ADJUSTED FOR 30.35 in  
ALCO TARGET *CS 7/14/09* .076 01:17  
BLANK TEST .000 01:18  
INTERNAL STANDARD VERIFIED 01:18  
ALCO TV 30.35 in .077 ✓ 01:18  
BLANK TEST .000 01:19  
SUBJECT SAMPLE *WTH* .000 01:20  
BLANK TEST *WTH* .000 01:21  
ALCO TV 30.35 in .078 ✓ 01:21  
BLANK TEST .000 01:22

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130188

JULY 07, 2009 ✓  
TIME 01:12

*WTH*

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 30.33 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢