

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130188</u> ✓	
Name		<u>HUTT, William T.</u>	ID# <u>3359</u> Date <u>09/04/08</u> ✓	
A	Agency	<u>AST/Anchor Point Post (ANPE)</u>	Phone # <u>235-8239</u> <u>235-3000</u>	
Instrument Location		<u>34115 Sterling Hwy. / P.O. Box 807</u> <u>Anchor Point, AK 99556</u> ✓		
Alco S/N		<u>X301536</u> ✓	Target Value <u>.075</u> ✓ High Pressure <u>400psi</u>	
B	Alco Test Value Average		<u>.070</u> ✓ 1 st Alco	<u>.070</u> ✓ 2 nd Alco
Signature		<u>William T. Hutt</u> ✓	<u>CSB</u> <u>9/11/08</u>	

(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, William Hutt, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

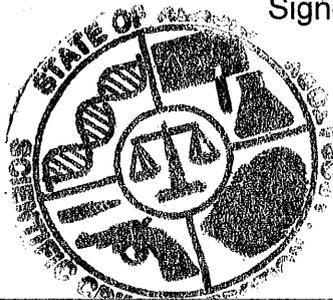

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

9/11/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130180 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

SEPTEMBER 04, 2000 *WTH*

OPERATOR'S NAME:
HUTT, WILLIAM T
OPERATOR'S NUMBER: 3359
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
ETOH

O.L. #: 01234567
DEPT/AGENCY: ASTO / ANPE
CASE/REPORT: 08-00000
TEST TYPE: V
ALCO TARGET VALUE: .075 ✓
ALCO S/N: X301536 ✓

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 30.32 in		
ALCO TARGET	.076	23:27
BLANK TEST	.000	23:27
INTERNAL STANDARD	VERIFIED	23:28
ALCO TV 30.32 in	.078 ✓	23:28
BLANK TEST	.000	23:29
SUBJECT SAMPLE <i>WTH</i>	.000 <i>WTH</i>	23:30
BLANK TEST	.000	23:31
ALCO TV 30.32 in	.078	23:31
BLANK TEST	.000	23:32

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130180

SEPTEMBER 04, 2000 ✓ *WTH*
TIME 23:23

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01

HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c

BAROMETER: 30.32 in

FLOW DETECTOR: OKAY

PUMP
HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ\]^_`ab cde fghijklmno
pqrstuvwxy z{|}~