

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

JUN 03 2010

Supervisor/Operator Performing the Verification Procedure:	
Name <u>Richard Eaton</u>	ID# <u>7287</u> Date <u>5/30/10</u>
Agency <u>St. Paul Island</u>	Phone # <u>907-546-3130</u>
Instrument Location <u>City Hall</u>	
DataMaster cdm S/N <u>130189</u>	
Alco S/N <u>X17299</u>	Target Value <u>.080</u> High Pressure <u>1700 psi</u>
Alco Test Values	<u>.082</u> <u>.081</u>
1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature <u>Richard B Eaton</u>	

(OVER)

BMB  
6/23/10

(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2<sup>nd</sup> day of July, 2010.

Carolyn M. Noland (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

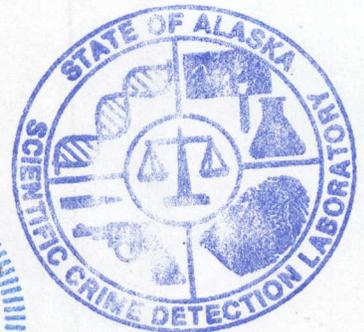

Target value not programmed. Breath  
Personnel needed to authenticate for court

BMB 6/23/10

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130189 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130189  
MAY 30, 2010 ✓  
OPERATOR'S NAME: *BMMB 6/23/10*  
EATON/RICHARD/B  
OPERATOR'S NUMBER: 7287  
SUBJECT'S LAST NAME:  
UOC  
SUBJECT'S FIRST NAME/MI :  
UOC  
O.L. #: 000000  
DEPT/AGENCY: SNP1  
CASE/REPORT: 000000  
TEST TYPE: U  
ALCO TARGET VALUE: .000 ✓  
ALCO S/N: X172991 ✓

### BREATH ANALYSIS

*BMMB 6/23/10*  
.001 ADJUSTED FOR 29.93 in  
ALCO TARGET .001 20:31  
BLANK TEST .000 20:32  
INTERNAL STANDARD VERIFIED 20:32  
ALCO TV 29.93 in .002 20:32  
BLANK TEST .000 20:33  
SUBJECT SAMPLE .000 20:34  
BLANK TEST .000 20:34  
ALCO TV 29.93 in .001 20:35  
BLANK TEST .000 20:35

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130189 ✓  
MAY 30, 2010 ✓  
TIME 20:28 ✓

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.93 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!@#%&'()\*+,-./0123456789:;<=>?@BCDEFG  
HIJKL MNOPQRSTUVWXYZ[\]^\_`ab cde fgh i jk l m n o  
p q r s t u v w x y z 1 2 3 4 5 6 7 8 9 0