

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130190</u> ✓
A	Name	<u>STEVE DUNN</u>	ID# <u>4106</u> Date <u>9-9-08</u> ✓
	Agency	<u>APD</u>	Phone # <u>786-8900</u>
	Instrument Location	<u>ANCHORAGE JAIL</u> ✓	
B	Alco S/N	<u>X301755</u> ✓	Target Value <u>.075</u> ✓ High Pressure <u>1200</u>
	Alco Test Value Average	<u>.074</u> ✓ 1 st Alco	<u>.074</u> ✓ 2 nd Alco
	Signature		<u>CDB</u> <u>9/12/08</u>
(OVER)			


Under the Alaska Rules of Evidence, I certify that:
(Do Not write in the area below)

(a) I am Jeane Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Steve P Dunn, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

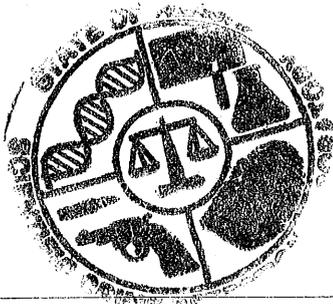

Handwritten signature of Jeane Swartz.

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

9/15/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130190 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

S. Dunn #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130190

SEPTEMBER 09, 2008 ✓
9/12/08

OPERATOR'S NAME:
DUNN/S
OPERATOR'S NUMBER: 4106
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
V
O.L. #: V
DEPT/AGENCY: ANC1
CASE/REPORT: V
TEST TYPE: V
ALCO TARGET VALUE: .075 ✓
ALCO S/N: K301755 ✓

--- BREATH ANALYSIS ---

.075 ADJUSTED FOR 29.80 in
ALCO TARGET .074 12:15
BLANK TEST .000 12:16
INTERNAL STANDARD VERIFIED 12:16
ALCO TV 29.80 in .074 ✓ 12:16
BLANK TEST .000 12:17
SUBJECT SAMPLE .000 ✓ 12:18
BLANK TEST .000 12:19
ALCO TV 29.81 in .074 ✓ 12:19
BLANK TEST .000 12:20

DIAGNOSTIC CHECK

S. Dunn #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130190

SEPTEMBER 09, 2008 ✓
TIME 12:11

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 02/20/01
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.80 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmnop
qrstuvwxyz{|}~