

VERIFICATION OF CALIBRATION REPORT ^{MAR 2 2009}
of DataMaster cdm Breath Test Instrument ^{MAR 2 2009}

State of Alaska

MAR 12 2009 Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130191 ✓
Name JOHN BENNETT ID# 4084 Date 3-12-09 ✓
A Agency ANCHORAGE POLICE DEPT. Phone # 786-8645
Instrument Location SEELY SUB-STATION, SPENARD RD. ✓
B Alco S/N 31085 ✓ Target Value .080 ✓ High Pressure 1000
Alco Test Values .083 ✓ .084 ✓
1st Alco 2nd Alco
Signature [Signature] ✓ CSB 3/27/09
(OVER)

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, John Bennett, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

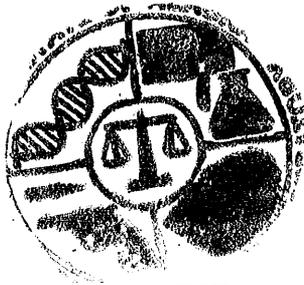

[Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

3/28/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska


Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130191

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

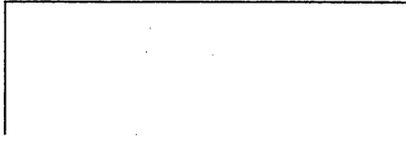

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191


MARCH 12, 2009 ✓

OPERATOR'S NAME:
BENNETT, JOHN
OPERATOR'S NUMBER: 4084
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
VOC


O.L. #: VOC
DEPT/AGENCY: ANCL
CASE/REPORT: VOC
TEST TYPE: V
ALCO TARGET VALUE: .080 ✓
ALCO S/N: 31085 ✓

--- BREATH ANALYSIS ---

.080 ADJUSTED FOR 29.86 in
ALCO TARGET .079 10:45
BLANK TEST .000 10:46
INTERNAL STANDARD VERIFIED 10:46
ALCO TV 29.86 in .083 10:46
BLANK TEST .000 ✓ 10:47
SUBJECT SAMPLE .000 ✓ 10:48
BLANK TEST .000 ✓ 10:48
ALCO TV 29.86 in .084 ✓ 10:49
BLANK TEST .000 10:50



DIAGNOSTIC CHECK



ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191

MARCH 12, 2009 ✓
TIME 10:53

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 12/11/08
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 42c
BAROMETER: 29.86 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
! "#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~`

