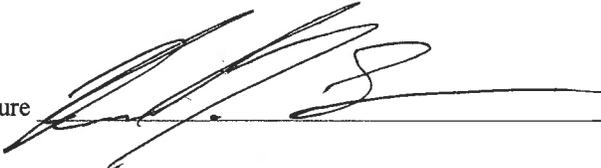


VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130191</u> ✓	
Name <u>BRANDON LAWRENSEN</u>		ID# <u>6609</u>	Date <u>9/30/10</u> ✓
A	Agency <u>JUNEAU POLICE</u>	Phone # <u>586-01600</u>	
Instrument Location <u>JUNEAU POLICE DEPT</u>			
Alco S/N ^{AL} <u>B-124646</u> ✓		Target Value <u>.077</u> ✓	High Pressure <u>400</u>
Alco Test Values		<u>.085</u> ✓ 1 st Alco	<u>.086</u> ✓ 2 nd Alco
Signature 			

(OVER)

BMB
10/5/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


 Nita J. Bolz
 Scientific Director
 State Breath Alcohol Program

Subscribed and sworn before me this 13 day of October 2010.



ba  (Notary Seal Stamp)
 Daniel L. Nicrotas
 Notary Public, State of Alaska
 Commission Expires with Office

BERTHA P. ANGNABOOGUK
 Notary Public, State of Alaska
 Commission # 108583
 My Commission Expires
 With Office

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130191

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191

SEPTEMBER 30, 2010

OPERATOR'S NAME:
LAWRENSEN/BRANDON/J
OPERATOR'S NUMBER: 6609
SUBJECT'S LAST NAME:

VOC
SUBJECT'S FIRST NAME/MI :
VOC

O.L. #: 0123456
DEPT/AGENCY: JNUL
CASE/REPORT: 0123456
TEST TYPE: V
ALCO TARGET VALUE: .077
ALCO S/N: X124646

--- BREATH ANALYSIS ---

.077 ADJUSTED FOR 30.04 in
ALCO TARGET .077 13:37
BLANK TEST .000 13:38
INTERNAL STANDARD VERIFIED 13:38
ALCO TV 30.04 in .085 13:38
BLANK TEST .000 13:39
SUBJECT SAMPLE .000 13:39
BLANK TEST .000 13:40
ALCO TV 30.04 in .086 13:40
BLANK TEST .000 13:41

BMB
10/5/10

BMB
10/5/10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191

SEPTEMBER 30, 2010
TIME 13:35

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/08/09
HEATERS
SAMPLE CHAMBER: 50c
BREATH TUBE: 41c
BAROMETER: 30.06 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNPOQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~*~