

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

| | | |
|--|---------------------------------------|--|
| Supervisor/Operator Performing the Verification Procedure: | | DataMaster cdm S/N <u>130191</u> ✓ |
| Name | <u>J Swartz</u> | ID# <u>4314</u> Date <u>12/29/08</u> ✓ |
| A Agency | <u>SCDL</u> | Phone # <u>269-5592</u> |
| Instrument Location | <u>SCDL</u> ✓ | |
| B Alco S/N | <u>SCOTT05</u> | Target Value <u>.080</u> ✓ High Pressure <u>1000 psi</u> |
| Alco Test Values | <u>.082</u> ✓ 1 st Alco | <u>.081</u> ✓ 2 nd Alco |
| Signature | <u>J Swartz</u> ✓ | <u>cos</u> <u>1/20/09</u> |

(OVER)


Under the Alaska Rules of Evidence, I certify that (Do not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jeanne M Swartz, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

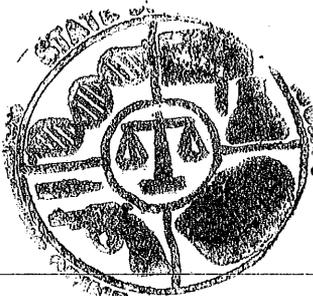

J Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

2/3/09

Date

BT9 06/03 JAN 13 2009

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130191

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191

DECEMBER 29, 2008 ✓

OPERATOR'S NAME:

SWARTZ/J

OPERATOR'S NUMBER: 4314

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

L

O.L. #: L

DEPT/AGENCY: AAA1

CASE/REPORT:

TEST TYPE: Y

ALCO TARGET VALUE: .000 ✓

ALCO S/N: SCOTT08 ✓

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.85 in

ALCO TARGET .079 18:12

BLANK TEST .000 18:13

INTERNAL STANDARD VERIFIED 18:13

ALCO TV 29.85 in .002 ✓ 18:13

BLANK TEST .000 18:14

SUBJECT SAMPLE .000 18:15

BLANK TEST .000 18:15

ALCO TV 29.85 in .001 18:16

BLANK TEST .000 18:16

J 12/29/08

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191

DECEMBER 29, 2008 ✓

TIME 18:08

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 12/11/08

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 42c

BAROMETER: 29.85 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

! " # % & ' () * + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G
H I J K L M N O P Q R S T U V W X Y Z [\] ^ _ ` a b c d e f g h i j k l m n o
p q r s t u v w x y z { | } ~