

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130191 ✓
Name		C. RITALA	ID# 3791 Date 12/29/08 ✓
A	Agency	A.P.D.	Phone # 786-2640
Instrument Location		Seely Sub (SPENARD)	✓
Alco S/N		X172966 ✓	Target Value -078 ✓ High Pressure 900
Alco Test Value Average		.084 ✓	.084 ✓
		1 st Alco	2 nd Alco
Signature		Chris Ritala ✓	1349
			COB 1/6/09

(OVER)


Under the Alaska Rules of Evidence, I certify that: (Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Chris Ritala, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed,

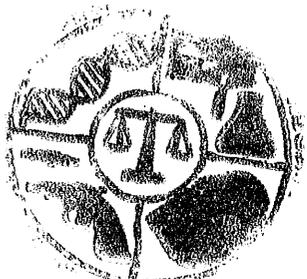

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

1/6/09

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130191 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191
DECEMBER 29, 2008
OPERATOR'S NAME: *CRS*
RITALA *11/6/09*
OPERATOR'S NUMBER: 3791
SUBJECT'S LAST NAME:
VERIFICATION OF CALIBRATION
SUBJECT'S FIRST NAME/NI :
A
O.L. #: A
DEPT/AGENCY: ANC1
CASE/REPORT: A
TEST TYPE: V
ALCO TARGET VALUE: .078 ✓
ALCO S/N: X172966
--- BREATH ANALYSIS ---
..078 ADJUSTED FOR 30.03 in
ALCO TARGET .078 18:51
BLANK TEST .000 18:51
INTERNAL STANDARD VERIFIED 18:51
ALCO TV 30.03 in .084 ✓ 18:52
BLANK TEST .000 18:52
SUBJECT SAMPLE *CRS* .000 18:54
BLANK TEST *11/6/09* .000 18:55
ALCO TV 30.03 in .084 ✓ 18:55
BLANK TEST .000 18:55
CR/12/29/08

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130191
DECEMBER 29, 2008 ✓
TIME 18:56
--- DIAGNOSTIC CHECK ---
COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 12/11/08
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 30.03 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY
PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJ
KLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~
CR/12/29/08