

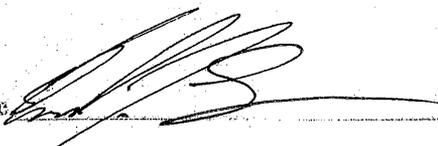
NOV 26 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster edm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster edm S/N <u>130192</u> ✓
Name	<u>BRANDON LAWRENSEN</u>	ID# <u>6609</u> Date <u>11/23/08</u> ✓
A Agency	<u>JUNEAU POLICE DEPT</u>	Phone # <u>586-0600</u>
Instrument Location	<u>JUNEAU POLICE DEPT</u> ✓	
B Alco S/N	<u>X124623</u> ✓	Target Value <u>.081</u> ✓ High Pressure <u>6000</u> ✓
Alco Test Values	<u>.083</u> ✓ 1 st Alco	<u>.083</u> ✓ 2 nd Alco
Signature	 ✓	
(OVER)		

Under the Alaska Rules of Evidence, I certify that, (Do not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Brandon Lawrenson, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.



Signed and sealed



 Jeanne Swartz
 Scientific Director, Designee
 State of Alaska
 State Breath Alcohol Testing Program

12/2/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster edm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster edm S/N 130192 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130192

NOVEMBER 23, 2008 ✓ *8/12/08*

OPERATOR'S NAME:
LAWRENSON/BRANDON/J
OPERATOR'S NUMBER: 6609
SUBJECT'S LAST NAME:
VOC
SUBJECT'S FIRST NAME/MI :
VOC
O.L. #: 0123456
DEPT/AGENCY: JNU1
CASE/REPORT: 012345
TEST TYPE: V
ALCO TARGET VALUE: .081 ✓
ALCO S/N: X124623

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 29.65 in		
ALCO TARGET	.080	15:31
BLANK TEST	.000	15:32
INTERNAL STANDARD	VERIFIED	15:32
ALCO TV 29.65 in	.083	15:32
BLANK TEST	.000 ✓	15:33
SUBJECT SAMPLE <i>8/12/08</i>	.000	15:33
BLANK TEST	.000	15:34
ALCO TV 29.64 in	.083 ✓	15:35
BLANK TEST	.000	15:35

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER edm 130192

NOVEMBER 23, 2008 ✓
TIME 15:42

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	42c
BAROMETER:	29.64 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefghijklmnop
qrstuvwxyz{|}~*~