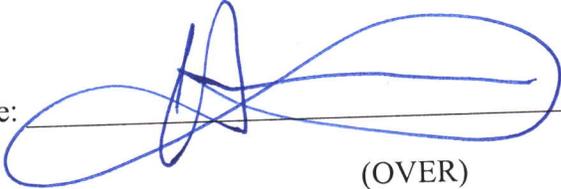


# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

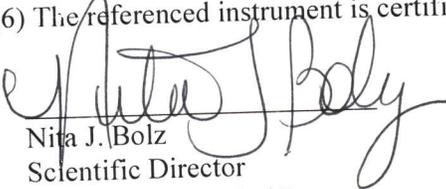
State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program


DataMaster cdm S/N: <u>130193</u>	
Supervisor/Operator Performing the Verification Procedure: Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>03 March 10</u>	
<b>A</b>	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>
Instrument Location: <u>Palmer Police Department</u>	
Alco S/N: <u>77621</u> Target Value: <u>.079</u> High Pressure: <u>925</u>	
<b>B</b>	Alco Test Value Average: $\frac{.079}{1^{st} \text{ Alco}}$ $\frac{.078}{2^{nd} \text{ Alco}}$
Signature:  (OVER) <span style="float: right;"><u>CB</u> <u>3/11/10</u></span>	

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of March, 2010.

 (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: ~~130298~~ <sup>130193</sup>

3/5/19  
CW

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193 ✓

MARCH 03, 2010 ✓

OPERATOR'S NAME: GIPSON/JAMES/C  
OPERATOR'S NUMBER: 4842  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: RJC68  
O.L. #: 0123456  
DEPT/AGENCY: PLM1  
CASE/REPORT: 01-2345  
TEST TYPE: U  
ALCO TARGET VALUE: .079 ✓  
ALCO S/N: 77621 ✓

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.05 in  
ALCO TARGET .076 13:59  
BLANK TEST .000 14:00  
INTERNAL STANDARD VERIFIED 14:00  
ALCO TV 29.05 in .079 ✓ 14:00  
BLANK TEST .000 14:01  
SUBJECT SAMPLE .000 14:04  
BLANK TEST .000 ✓ 14:04  
ALCO TV 29.05 in .078 ✓ 14:05  
BLANK TEST .000 14:05

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193 ✓

MARCH 03, 2010 ✓  
TIME 13:56

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 43c  
BAROMETER: 29.03 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST  
!\*"#%&'()\*+,-./0123456789:;<=>?@ABCDEFGHIJKL  
HIJKLMNPOQRSTUVWXYZ[\]^\_`abcdefgijklmnop  
qrstuvwxyz{|}~`