

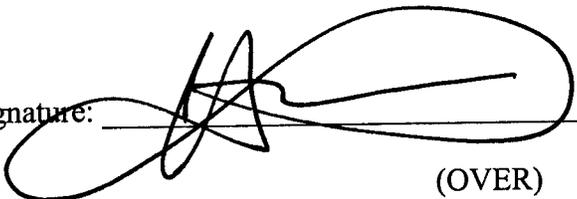
VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

SEP 10 2009

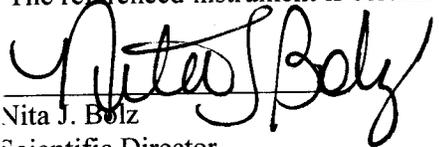
Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure: Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>28 August 09</u> ✓		DataMaster cdm S/N: <u>130193</u> ✓
A	Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>	
	Instrument Location: <u>Palmer Police Department</u> ✓	
B	Alco S/N: <u>X172946</u> ✓ Target Value: <u>.077</u> ✓ High Pressure: <u>1100</u>	
	Alco Test Value Average: <u>.077</u> <u>.075</u> 1 st Alco 2 nd Alco	
	Signature: 	
	(OVER)	

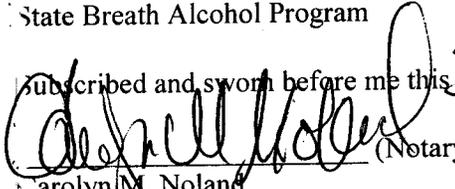
BMB
9/22/09

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

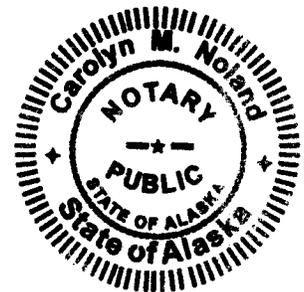
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 15 day of Oct, 2009.


(Notary Seal Stamp)

Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298

130193 ^{BMB} 9/22/09

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130193

AUGUST 28, 2009

OPERATOR'S NAME:
GIPSON/JAMES/C
OPERATOR'S NUMBER: 4842
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
RJCS0

O.L. #: 0123456
DEPT/AGENCY: PLH1
CASE/REPORT: 01-2345
TEST TYPE: U
ALCO TARGET VALUE: .077 ✓
ALCO S/N: X172946 ✓

— BREATH ANALYSIS —

.077 ADJUSTED FOR 29.59 in
ALCO TARGET .076 15:37
BLANK TEST .000 15:38
INTERNAL STANDARD VERIFIED 15:38
ALCO TV 29.59 in .077 ✓ 15:39
BLANK TEST .000 15:39
SUBJECT SAMPLE .000 15:40
BLANK TEST .000 15:41
ALCO TV 29.59 in .075 ✓ 15:41
BLANK TEST .000 15:42

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130193 ✓

AUGUST 28, 2009
TIME 15:29

— DIAGNOSTIC CHECK —

COMPUTER: OKAY
PROGRAM: OKAY
SOFTWARE DATE: 01/00/09
HEATERS
SAMPLE CHAMBER: 49c
BREATH TUBE: 41c
BAROMETER: 29.60 in
FLOW DETECTOR: OKAY
PUMP
HIGH SPEED: OKAY
DETECTOR: OKAY
FILTERS: OKAY
QUARTZ STANDARD: OKAY
CALIBRATION: OKAY

PRINTER TEST
!"#\$%&'()*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcdefgijklmno
pqrstuvwxyz{|}~■