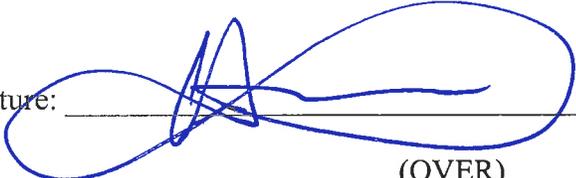


VERIFICATION OF CALIBRATION REPORT SEP 09 2010

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N: <u>130193</u> ✓
Name: <u>JAMES C. GIPSON</u>	ID#: <u>4842</u> ✓	Date: <u>9/2/10</u> 02 Aug 10 ^{omj} 9/8/10
Agency: <u>Palmer Police Department</u>		Phone #: <u>(907) 745-4811</u>
Instrument Location: <u>Palmer Police Department</u>		
Alco S/N: <u>718493</u> ✓ Target Value: <u>.084</u> ✓ High Pressure: <u>825</u>		
Alco Test Value Average: <u>.085</u> ✓ 1 st Alco 2 nd Alco		
Signature: 		

(OVER)

Handwritten initials and date:
DWB
9/10/10

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 27th day of Oct, 2010.


Daniel L. Nicholas
Notary Public, State of Alaska
Commission Expires with Office

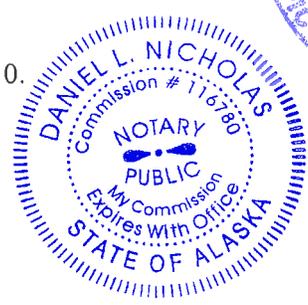

VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

DataMaster cdm S/N: 130193

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130193

SEPTEMBER 02, 2010

OPERATOR'S NAME:
DIPSON/JAMES/C

OPERATOR'S NUMBER: 4842

SUBJECT'S LAST NAME:
VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :
RJCSB

O.L. #: 0123456
DEPT/AGENCY: PLM1
CASE/REPORT: 01-2345
TEST TYPE: U
ALCO TARGET VALUE: .084
ALCO S/N: 710497

--- BREATH ANALYSIS ---

.084 ADJUSTED FOR 29.81 in		
ALCO TARGET	.083	14:41
BLANK TEST	.000	14:42
INTERNAL STANDARD	VERIFIED	14:42
ALCO TU 29.81 in	.085	14:42
BLANK TEST	.000	14:43
SUBJECT SAMPLE	.000	14:44
BLANK TEST	.000	14:45
ALCO TU 29.81 in	.084	14:45
BLANK TEST	.000	14:46

BMB 9/10/10

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130193

SEPTEMBER 02, 2010
TIME 14:46

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 29.81 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@BCDEFG
HIJKLMNOPQRSTUVWXYZ\]^_`ab|cde|fghi|jklmno
pqrs|tuvwxyz{|}~■