

# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

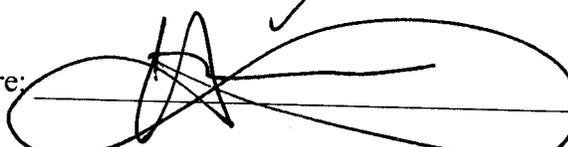
Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

NOV 23 2009

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N: 130193 ✓  
Name: JAMES C. GIPSON ID#: 4842 Date: 21 BMB 12/11/09 ✓  
**A** Agency: Palmer Police Department Phone #: (907) 745-4811  
Instrument Location: Palmer Police Department

---

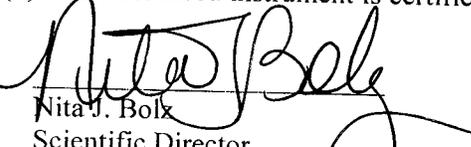
Alco S/N: X124671 Target Value: 0.084 <sup>BMB</sup> ~~0.076~~ <sup>12/23/09 \*</sup> High Pressure: 1250  
**B** Alco Test Value Average: 0.084 <sup>1st Alco</sup> 0.083 <sup>2nd Alco</sup> <sup>\* Target value corrected at Lab 12/23/09 BMB</sup>

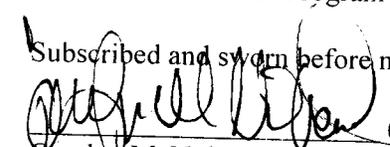
Signature:  (OVER)


<sup>BMB</sup>  
<sup>12/23/09</sup>

I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 21 day of Jan. 2010  
 (Notary Seal Stamp) 2009  
1-8-10  
CW



# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N: 130298

130193  
11-23-09  
cmw

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

NOVEMBER 21, 2009

OPERATOR'S NAME: GIPSON, JAMES/C  
OPERATOR'S NUMBER: 4942  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: RJCS0  
O.L. #: 0123456  
DEPT/AGENCY: PLM1  
CASE/REPORT: 01-2345  
TEST TYPE: U  
ALCO TARGET VALUE: .076  
ALCO S/N: X124671

BMB  
12/23/09

\* 0.084  
BMB  
12/23/09

--- BREATH ANALYSIS ---

.076 ADJUSTED FOR 29.42 in		
ALCO TARGET	.074	23:17
BLANK TEST	.000	23:17
INTERNAL STANDARD	VERIFIED	23:17
ALCO TU 29.41 in	.084	23:18
BLANK TEST	.000	23:18
SUBJECT SAMPLE	.000	23:19
BLANK TEST	.000	23:20
ALCO TU 29.41 in	.083	23:20
BLANK TEST	.000	23:21

\* Target value corrected at lab  
0.084  
BMB  
12/23/09  
recalculated  
NJB  
11/7/10

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193

NOVEMBER 21, 2009  
TIME 23:08

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.42 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; < = > ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z [ \ ] ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢