

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130195

Supervisor/Operator Performing the Verification Procedure:

**A**  
Name Robert J. Ely ID# 2681 Date 06-07-2012  
Agency Craig Police Department Phone # (907) 826-3330  
Instrument Location 506 2<sup>nd</sup> Street, Craig Alaska 99921

**B**  
Alco S/N 75509 Target Value .079 High Pressure 250 PSI  
Alco Test Value Average .080  
1<sup>st</sup> Alco .080 2<sup>nd</sup> Alco

Signature *Robert J. Ely*

(OVER)

(Do Not write in the area below)

*MB*  
*6/14/12*


I, Nita J. Bolz, after being first duly sworn, depose and state as follows;

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons Responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska

*Nita J. Bolz*  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 3rd day of July, 2012 *NAC 7/3/12*

*Nikki Roth* (Notary Seal Stamp)  
*NAC*  
~~Daniel L. Nicholas~~ Nikki Roth  
Notary Public, State of Alaska  
Commission Expires with Office  
*7/3/12*

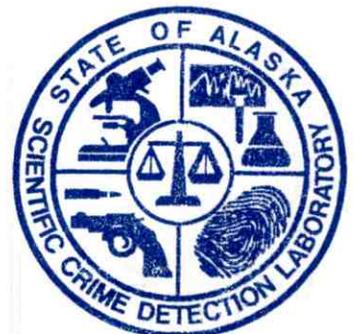

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130195

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130195

JUNE 07, 2012

OPERATOR'S NAME:

ELY, RJ

OPERATOR'S NUMBER: 2681

SUBJECT'S LAST NAME:

VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :

VER OF CAL

O.L. #: 123456789

DEPT/AGENCY: CRG1

CASE/REPORT: 12-0633X

TEST TYPE: U

ALCO TARGET VALUE: .079

ALCO S/N: 75509

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.88 in  
ALCO TARGET .078 14:47  
BLANK TEST .000 14:47  
INTERNAL STANDARD VERIFIED 14:48  
ALCO TV 29.88 in .000 14:48  
BLANK TEST .000 14:49  
SUBJECT SAMPLE .000 14:50  
BLANK TEST .000 14:50  
ALCO TV 29.88 in .000 14:51  
BLANK TEST .000 14:51

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130195

JUNE 07, 2012

TIME 14:45

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 02/20/01  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 42c  
BAROMETER: 29.88 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

PRINTER TEST

! " # \$ % & ' ( ) \* + , - . / 0 1 2 3 4 5 6 7 8 9 : ; ( = ) ? @ A B C D E F G  
H I J K L M N O P Q R S T U V W X Y Z I \ ^ \_ ` a b c d e f g h i j k l m n o  
p q r s t u v w x y z { | } ~ ¡ ¢

