

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130195</u> ✓	
Supervisor/Operator Performing the Verification Procedure:	
A Name <u>Robert J. Ely</u>	ID# <u>2681</u> Date <u>12-31-2008</u> ✓
Agency <u>Craig Police Department</u>	Phone # <u>(907) 826-3330</u>
Instrument Location <u>506 2nd Street, Craig Alaska 99921</u>	✓
Alco S/N <u>77286</u> ✓	Target Value <u>.079</u> ✓ High Pressure <u>500</u> PSI
Alco Test Value Average <u>.083</u> ✓	<u>.083</u> ✓
1 st Alco	2 nd Alco
Signature <u>Robert J. Ely</u>	<u>CS</u> <u>1/30/09</u>
(OVER)	

(Do Not write in the area below)


Under the Alaska Rules of Evidence, I certify that;

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Robert J Ely, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

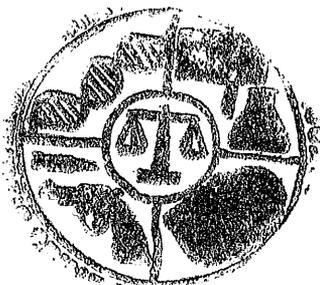

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

2/3/09
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130195

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130195

DECEMBER 31, 2008

OPERATOR'S NAME: *QCB 1/20/09*
Ely, RJ
OPERATOR'S NUMBER: 2681
SUBJECT'S LAST NAME:
VERIFICATION OF CAL
SUBJECT'S FIRST NAME/MI :
VER OF CAL
O.L. #: 123456789
DEPT AGENCY: CRG1
CASE/REPORT: 00-XXXX
TEST TYPE: U
ALCO TARGET VALUE: .079 ✓
ALCO S/N: 77236

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.99 in		
ALCO TARGET	.079	16:50
BLANK TEST	.000	16:50
INTERNAL STANDARD	VERIFIED	16:50
ALCO TU 29.99 in	.083	16:51
BLANK TEST	.000	16:52
SUBJECT SAMPLE	.000	16:52
BLANK TEST	.000	16:53
ALCO TU 29.99 in	.083	16:53
BLANK TEST	.000	16:54

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130195

DECEMBER 31, 2008 ✓
TIME 16:48

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	43c
BAROMETER:	29.99 in
FILM DETECTOR:	OKAY
PUMP	
RPM SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!@#\$%^&*+,-./0123456789:;<=>?@ABCDEF
GHIJKLMNOPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxy z{|}~#