

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:	
DataMaster cdm S/N <u>130196</u>	
Name	<u>JEAN P. ACHEE</u> ID# <u>1470</u> Date <u>7/3/2008</u> ✓
A Agency	<u>WASILLA POLICE DEPT.</u> Phone # <u>352-5401</u>
Instrument Location	<u>WASILLA POLICE DEPT.</u> ✓
B Alco S/N	<u>X301568</u> ✓ Target Value <u>.071</u> ✓ High Pressure <u>1300</u> ✓
Alco Test Value Average	<u>.077</u> <u>.079</u> 1 st Alco 2 nd Alco
Signature	<u>Jean Achee</u>
(OVER)	

Under the Alaska Rules of Evidence, I certify that;
(Do Not write in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Jean P Achee, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

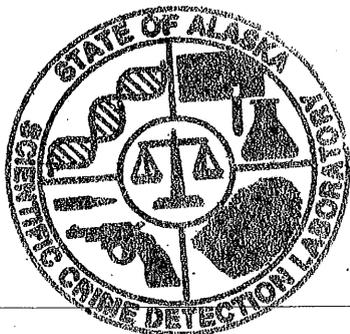

Signed and sealed,

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

7/13/08
Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130196

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130196

JULY 03, 2008

OPERATOR'S NAME:

ACHEE, JEAN P

OPERATOR'S NUMBER: 1470

SUBJECT'S LAST NAME:

VOC

SUBJECT'S FIRST NAME/MI :

VOC

O.L.L. #: 1234567890

DEPT/AGENCY: MASI

CASE/REPORT: 00-0703

TEST TYPE: V

ALCO TARGET VALUE: .072 ✓

ALCO S/N: X301568 ✓

--- BREATH ANALYSIS ---

.072 ADJUSTED FOR 29.52 in

ALCO TARGET	.071	17:58
BLANK TEST	.000	17:58
INTERNAL STANDARD	VERIFIED	17:59
ALCO TV 29.52 in	.077 ✓	17:59
BLANK TEST	.000	18:00
SUBJECT SAMPLE	.000	18:01
BLANK TEST	.000	18:01
ALCO TV 29.52 in	.079 ✓	18:02
BLANK TEST	.000	18:03

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130196

JULY 03, 2008 ✓

TIME 17:54

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 43c

BAROMETER: 29.52 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEFB
HIJKLMNPOQRSTUVWXYZ[\]^_`abcde fghi.jklmno
pqrs:tuvwxyz{|}~