

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

2009

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130196

Name Garrett Willis ID# 5560 Date 10/30/09

A Agency ASI Phone # 262-4453

Instrument Location Cooper Landing ASI

B Alco S/N 57345 Target Value .082 High Pressure 1,000

Alco Test Values .081 1<sup>st</sup> Alco .081 2<sup>nd</sup> Alco

Signature Garrett Willis

(OVER)

BMB  
11/4/09


(Do Not write in the area below)

- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

Nita J. Bolz  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 30<sup>th</sup> day of Dec, 2009.

Carolyn M. Noland (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

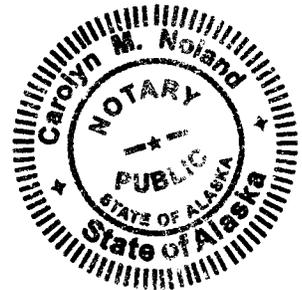

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130196

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130196 ✓  
OCTOBER 30, 2009 ✓ *Bomb 10/14/09*  
OPERATOR'S NAME: WILLIS/GARRETT/R  
OPERATOR'S NUMBER: 5560  
SUBJECT'S LAST NAME: VOC *GLW*  
SUBJECT'S FIRST NAME/NI: VOC  
O.L. #: VOC  
DEPT/AGENCY: COOB  
CASE/REPORT: VOC  
TEST TYPE: V  
ALCO TARGET VALUE: .082 ✓  
ALCO S/N: 57345 ✓

— BREATH ANALYSIS —

.082 ADJUSTED FOR 29.26 in		
ALCO TARGET	.000	13:29
BLANK TEST	.000	13:29
INTERNAL STANDARD	VERIFIED	13:30
ALCO TV 29.26 in	.081	13:30
BLANK TEST	.000	13:31
SUBJECT SAMPLE	.000	13:31
BLANK TEST	.000	13:32
ALCO TV 29.25 in	.081	13:32
BLANK TEST	.000	13:33

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130196 ✓  
OCTOBER 30, 2009 ✓  
TIME 13:26 ✓

— DIAGNOSTIC CHECK —

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	01/08/09
HEATERS	
SAMPLE CHAMBER:	49c
BREATH TUBE:	41c
BAROMETER:	29.25 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST  
!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMNOPQRSTUVWXYZ[\]^\_`abcdefgijklmno  
pqrstuvwxyz{|}~