

MAR 03 2008

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130287^v</u>
Name	<u>Mitch Langseth</u>	ID# <u>2612</u> Date <u>2/27/08</u>
A Agency	<u>KOT Kenai Police Dept</u>	Phone # <u>283-7879</u>
Instrument Location <u>Wildwood Patrol</u>		
B Alco S/N <u>58427^v</u> Target Value <u>.081^v</u> High Pressure <u>1000</u>		
Alco Test Value Average		
	<u>.079</u> 1 st Alco	<u>.080</u> 2 nd Alco
Signature <u>[Handwritten Signature]</u>		<u>[Handwritten Initials]</u> <u>9/6/08</u>


(OVER)

Under the Alaska Rules of Evidence, I certify that (write in the area below)

(a) I am Jeanne Swartz, Criminalist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Mitch E Langseth, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

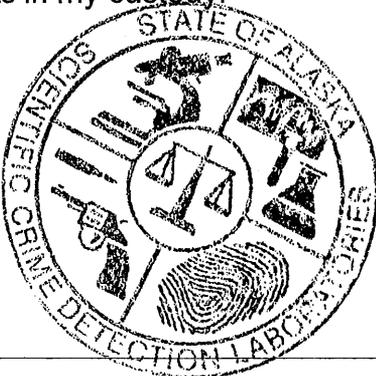

Signed and sealed

[Handwritten Signature]

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

03/07/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130287

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130287

FEBRUARY 27, 2008

OPERATOR'S NAME: *COB 3/6/08*
LANGSETH

OPERATOR'S NUMBER: 2612

SUBJECT'S LAST NAME:

VER OF CAL

SUBJECT'S FIRST NAME/NI :
NONE

O.L. #: 0

DEPT/AGENCY: KENI

CASE/REPORT: 0

TEST TYPE: U

ALCO TARGET VALUE: .001

ALCO S/N: 50427

--- BREATH ANALYSIS ---

8/17/08

.001 ADJUSTED FOR 29.80 in		
ALCO TARGET	.000	19:06
BLANK TEST	.000	19:07
INTERNAL STANDARD	VERIFIED	19:07
ALCO TV 29.80 in	.079	19:08
BLANK TEST	.000	19:09
SUBJECT SAMPLE	.000 <i>COB 3/6/08</i>	19:09
BLANK TEST	.000	19:10
ALCO TV 29.80 in	.000	19:10
BLANK TEST	.000	19:11

19:11

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130287

FEBRUARY 27, 2008

TIME 19:01

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	43c
BAROMETER:	29.80 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST

!"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJKL
MNPQRSTUVWXYZ[\]^_`abcde fghijklmno
pqrstuvwxyz{|}~!@