

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument  
State of Alaska

AUG 14 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N <u>130287</u>	
Supervisor/Operator Performing the Verification Procedure:	
Name <u>Mitchell E. Langseth</u>	ID# <u>2612</u> Date <u>8/6/09</u>
A Agency <u>Kenai Police Department</u> Phone # <u>907-283-7879</u>	
Instrument Location <u>Wildwood Pretrial Facility, Kenai Alaska</u>	
B Alco S/N <u>X301765</u> Target Value <u>.085</u> High Pressure <u>1270</u>	
Alco Test Value Average <u>.083</u>	<u>.084</u>
1 <sup>st</sup> Alco	2 <sup>nd</sup> Alco
Signature <u>[Handwritten Signature]</u>	<u>CSB</u> <u>8/24/09</u>
(OVER)	

(Do Not write in the area below)


- I, Nita J. Bolz, after being first duly sworn, depose and state as follows:
- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
  - (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
  - (3) I am the Scientific Director of the State Breath Alcohol Program.
  - (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
  - (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
  - (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Handwritten Signature: Nita J. Bolz]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 17<sup>th</sup> day of Sept, 2009.

[Handwritten Signature: Carolyn M. Noland] (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

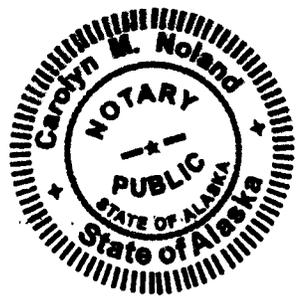

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130287 ✓

(CONTINUED FROM FRONT PAGE)

**C** TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130287 ✓  
AUGUST 06, 2009 ✓ *CBS 8/27/09*

OPERATOR'S NAME: LANGSETH  
OPERATOR'S NUMBER: 2612  
SUBJECT'S LAST NAME: TEST  
SUBJECT'S FIRST NAME/MI: VERIFICATION OF CAL  
O.L. #: 0  
DEPT/AGENCY: KENI  
CASE/REPORT: 0  
TEST TYPE: U  
ALCO TARGET VALUE: 0.05 ✓  
ALCO S/N: X301765 ✓

--- BREATH ANALYSIS ---

.005 ADJUSTED FOR 30.04 in		
ALCO TARGET	.005	15:17
BLANK TEST	.000	15:18
INTERNAL STANDARD	VERIFIED	15:18
ALCO TO 30.04 in	.003 ✓	15:19
BLANK TEST	.000	15:20
SUBJECT SAMPLE <i>8/27/09</i>	.000	15:20
BLANK TEST	.000	15:21
ALCO TO 30.04 in	.004 ✓	15:22
BLANK TEST	.000	15:23

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130287  
AUGUST 06, 2009 ✓  
TIME 15:14

--- DIAGNOSTIC CHECK ---

COMPUTER:	OKAY
PROGRAM:	OKAY
SOFTWARE DATE:	02/20/01
HEATERS	
SAMPLE CHAMBER:	48c
BREATH TUBE:	41c
BAROMETER:	30.04 in
FLOW DETECTOR:	OKAY
PUMP	
HIGH SPEED:	OKAY
DETECTOR:	OKAY
FILTERS:	OKAY
QUARTZ STANDARD:	OKAY
CALIBRATION:	OKAY

PRINTER TEST  
!#\$%&'()\*+,-./0123456789:;<=>@ABCDEFGHIJKL  
MNPQRSTUVWXYZ[\]^\_`abcdefgijklmnopqrstuvwxyz{|}~