

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N <u>130288</u> ✓	
Name	<u>DIXIE SPENCER</u>	ID#	<u>2280</u> Date <u>9/14/08</u> ✓
A Agency	<u>AST</u>	Phone #	<u>675-4398</u> ✓
Instrument Location <u>ANI AK</u> ✓			
Alco S/N <u>X301605</u> ✓		Target Value	<u>.079</u> ✓ High Pressure <u>1150</u>
Alco Test Values		<u>0.083</u>	<u>0.083</u>
		<u>83</u> ¹⁰⁰ / ₁₂₂₀₈	<u>83</u> ¹⁰⁰ / ₁₂₂₀₈
		1 st Alco	2 nd Alco
Signature <u>Dixie Spencer</u> ✓		<u>CS</u> <u>9/22/08</u>	

(OVER)


Under the Alaska Rules of Evidence, I ~~Certify that~~ (Certify that) in the area below)

(a) I am Jeanne Swartz, Forensic Scientist III, Scientific Crime Detection Laboratory, State of Alaska Department of Public Safety, and was, at the time of signing, the custodian of the records of the aforementioned laboratory and the signature was made in my official capacity as Scientific Director Designee of the State Breath Alcohol Testing Program.

(b) The verification of calibration for the above instrument has been received and reviewed. Instrument operator, Dixie Spencer, whose name appears in my records, is qualified to verify the calibration of the above instrument.

(c) This instrument is certified for evidentiary use and these records are being retained as original documents in my custody.

Signed and sealed

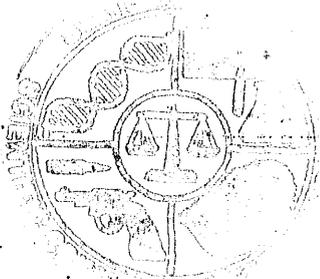

Jeanne Swartz

Jeanne Swartz
Scientific Director Designee
State of Alaska
State Breath Alcohol Testing Program

10/5/08

Date

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130288 ✓

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130288

SEPTEMBER 14, 2008 *cos 9/20/08*

OPERATOR'S NAME:

DIXIE SPENCER

OPERATOR'S NUMBER: 2200

SUBJECT'S LAST NAME:

FFFFFFF

SUBJECT'S FIRST NAME/MI:

KKKK

O.L. #: 000000

DEPT/AGENCY: ANTI0

CASE/REPORT: 00-

TEST TYPE: U

ALCO TARGET VALUE: .079 ✓

ALCO S/N: X301605 ✓

--- BREATH ANALYSIS ---

.079 ADJUSTED FOR 29.52 in
ALCO TARGET .077 15:01
BLANK TEST .000 15:02
INTERNAL STANDARD VERIFIED 15:02
ALCO TU 29.52 in .083 15:02
BLANK TEST .000 15:03
SUBJECT SAMPLE .000 *cos 9/20/08* 15:04
BLANK TEST .000 ✓ 15:05
ALCO TU 29.52 in .083 15:05
BLANK TEST .000 15:06

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
DATAMASTER cdm 130288 ✓

SEPTEMBER 14, 2008 ✓

TIME 15:18

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 43c

BAROMETER: 29.52 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!@#%&'()*+,-./0123456789:;<=>?@ABCDEF
HIJKLMNPQRSTUUVWXYZ\]^_`abcde fghijklmno
pqrstuvwxyz{|}~#