

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAR 11 2010

Supervisor/Operator Performing the Verification Procedure: DataMaster cdm S/N 130290

Name STEVE DUNN ID# 4106 Date 3-11-10

A Agency APD Phone # 764-1361

Instrument Location ANCHORAGE JAIL

B Alco S/N 1A Target Value .080 High Pressure 1000 PSF

Alco Test Value Average .079 .075

1<sup>st</sup> Alco 2<sup>nd</sup> Alco

Signature [Signature]

(OVER)

*BMB*  
*3/18/2010*



I, Nita J. Bolz, after being first duly sworn, depose and state as follows: (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

[Signature]  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 2<sup>nd</sup> day of April, 2010.

[Signature] (Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

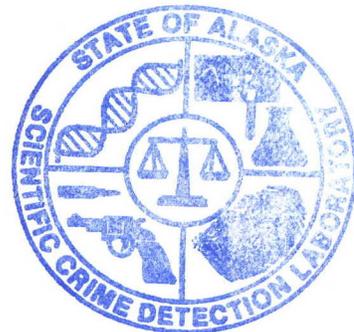

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130290

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

*S. DUNN \*1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130290

MARCH 11, 2010

OPERATOR'S NAME:  
DUNN/S

OPERATOR'S NUMBER: 4286

SUBJECT'S LAST NAME:  
VERIFICATION OF CAL

SUBJECT'S FIRST NAME/MI :  
V

O.L. #: V

DEPT/AGENCY: ANCI

CASE/REPORT: V

TEST TYPE: V

ALCO TARGET VALUE: .000 ✓

ALCO S/N: 1A

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 29.25 in ✓

ALCO TARGET	.078	09:50
BLANK TEST	.000	09:51
INTERNAL STANDARD	VERIFIED	09:51
ALCO TV 29.25 in	.079	09:52
BLANK TEST	.000	09:52
SUBJECT SAMPLE	.000	09:53
BLANK TEST	.000	09:54
ALCO TV 29.25 in	.075	09:54
BLANK TEST	.000	09:55

*BMB 3/18/2010*

## DIAGNOSTIC CHECK

*S. DUNN \*1361*

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130290 ✓

MARCH 11, 2010 ✓  
TIME 09:48 ✓

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 42c

BAROMETER: 29.25 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""%&'()\*+,-.0123456789:;<=>?@ABCDEFGHIJKL  
HIJKLMNOPQRSTUVWXYZ[-\_`abcde fghijklmno  
pqrstuvwxyz{|}~`