

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

MAY 2³ 2010

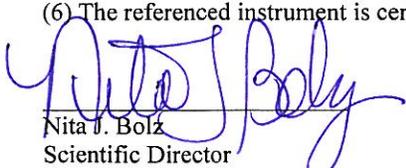
Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130290 130293 0086/110 ✓
Name		Troy Clark	ID# 4934 Date 5.29.10 ✓
A	Agency	Anchorage Police	Phone # 786.8900
Instrument Location		Jail, north processing room ✓	
Alco S/N		2C ✓	Target Value .080 ✓ High Pressure 1000
Alco Test Values		.079 ✓ 1 st Alco	.079 ✓ 2 nd Alco
Signature		Troy Clark ✓	003 6/10/10

(OVER)

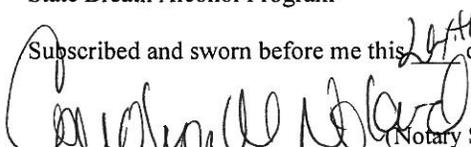
(Do Not write in the area below)

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.


Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 29th day of June 2010.


Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office

(Notary Seal Stamp)



VERIFICATION OF CALIBRATION REPORT
of DataMaster cdm breath Test Instrument
State of Alaska
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

130290
 DataMaster cdm S/N ~~130293~~ ^{COB 6/10/10}

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130293 ✓

MAY 29, 2010 ✓

OPERATOR'S NAME: *COB 6/10/10*
 CLARK/TROY

OPERATOR'S NUMBER: 4934

SUBJECT'S LAST NAME:
 VOC

SUBJECT'S FIRST NAME/MI :
 VOC

O.L. #: VOC

DEPT/AGENCY: ANCI

CASE/REPORT: 10-12345

TEST TYPE: V ✓

ALCO TARGET VALUE: .000 ✓

ALCO S/N: 20

--- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.19 in ✓

ALCO TARGET	.000	05:26
BLANK TEST	.000	05:27
INTERNAL STANDARD	VERIFIED	05:27
ALCO TV 30.19 in	.079 ✓	05:27
BLANK TEST	.000	05:28
SUBJECT SAMPLE <i>COB 6/10/10</i>	.000	05:28
BLANK TEST	.000	05:29
ALCO TV 30.19 in	.079 ✓	05:29
BLANK TEST	.000	05:30

DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY
 DATAMASTER cdm 130293 ✓

MAY 29, 2010 ✓
 TIME 05:15

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 01/08/09

HEATERS

SAMPLE CHAMBER: 49c

BREATH TUBE: 41c

BAROMETER: 30.19 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!*"#\$%&'()*+,-./0123456789:;<=>@ABCDEFGHIJ
 KL MNOPQRSTUVWXYZ_`~*abcdefghijklmnopqrstu
 vwxyz{|}~`