

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

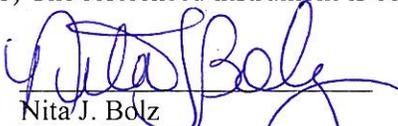
State of Alaska

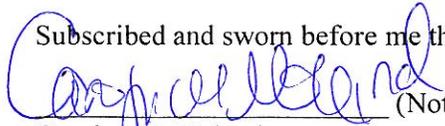
Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program


Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130290</u> ✓
A	Name	<u>STEVE DUNN</u>	ID# <u>4106</u> ✓ Date <u>6-22-10</u> ✓
	Agency	<u>APD</u>	Phone # <u>786-8900</u>
	Instrument Location	<u>ANCHORAGE JAIL</u>	
B	Alco S/N	<u>21</u> ✓	Target Value <u>.080</u> ✓ High Pressure <u>1100</u> PSI
	Alco Test Value Average	<u>.078</u> ✓ 1 <sup>st</sup> Alco	<u>.078</u> ✓ 2 <sup>nd</sup> Alco
Signature			
		COS 6/28/10	
(OVER)			

I, Nita J. Bolz, after being first duly sworn, depose and state as follows (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 26<sup>th</sup> day of July, 2010.  
  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130290

(CONTINUED FROM FRONT PAGE)

C TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293

JUNE 22, 2010 <sup>COB</sup>  
6/28/10

OPERATOR'S NAME: DUNN/S  
OPERATOR'S NUMBER: 4126  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: V  
O.L. #: V  
DEPT/AGENCY: ANCI  
CASE/REPORT: V  
TEST TYPE: V  
ALCO TARGET VALUE: .000  
ALCO S/N: 21

### --- BREATH ANALYSIS ---

.000 ADJUSTED FOR 30.09 in  
ALCO TARGET .000 11:26  
BLANK TEST .000 11:27  
INTERNAL STANDARD VERIFIED 11:27  
ALCO TV 30.09 in .078 11:27  
BLANK TEST .000 11:28  
SUBJECT SAMPLE .000 11:28  
BLANK TEST .000 11:29  
ALCO TV 30.09 in <sup>COB</sup> .078 11:29  
6/28/10  
BLANK TEST .000 11:30

## DIAGNOSTIC CHECK

S. DUNN #1361

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130293

JUNE 22, 2010  
TIME 11:24

### --- DIAGNOSTIC CHECK ---

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 30.09 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!"#\$%&'()\*+,-./0123456789:;<=>?@ABCDEF6  
HIJKLMN0PQRSTUWXYZ!:"\_ ' abcde fghijklmno  
pqrstuvwxyz(1)+~